


MED11103478710 2:26-03-2008 01 PM  
2322208182  
MR SAINI RAJANI (A Y/M)



9f CLUMAX DIAGNOSTICS THIRUPASANDRA BANGALOR

HR 80 bpm

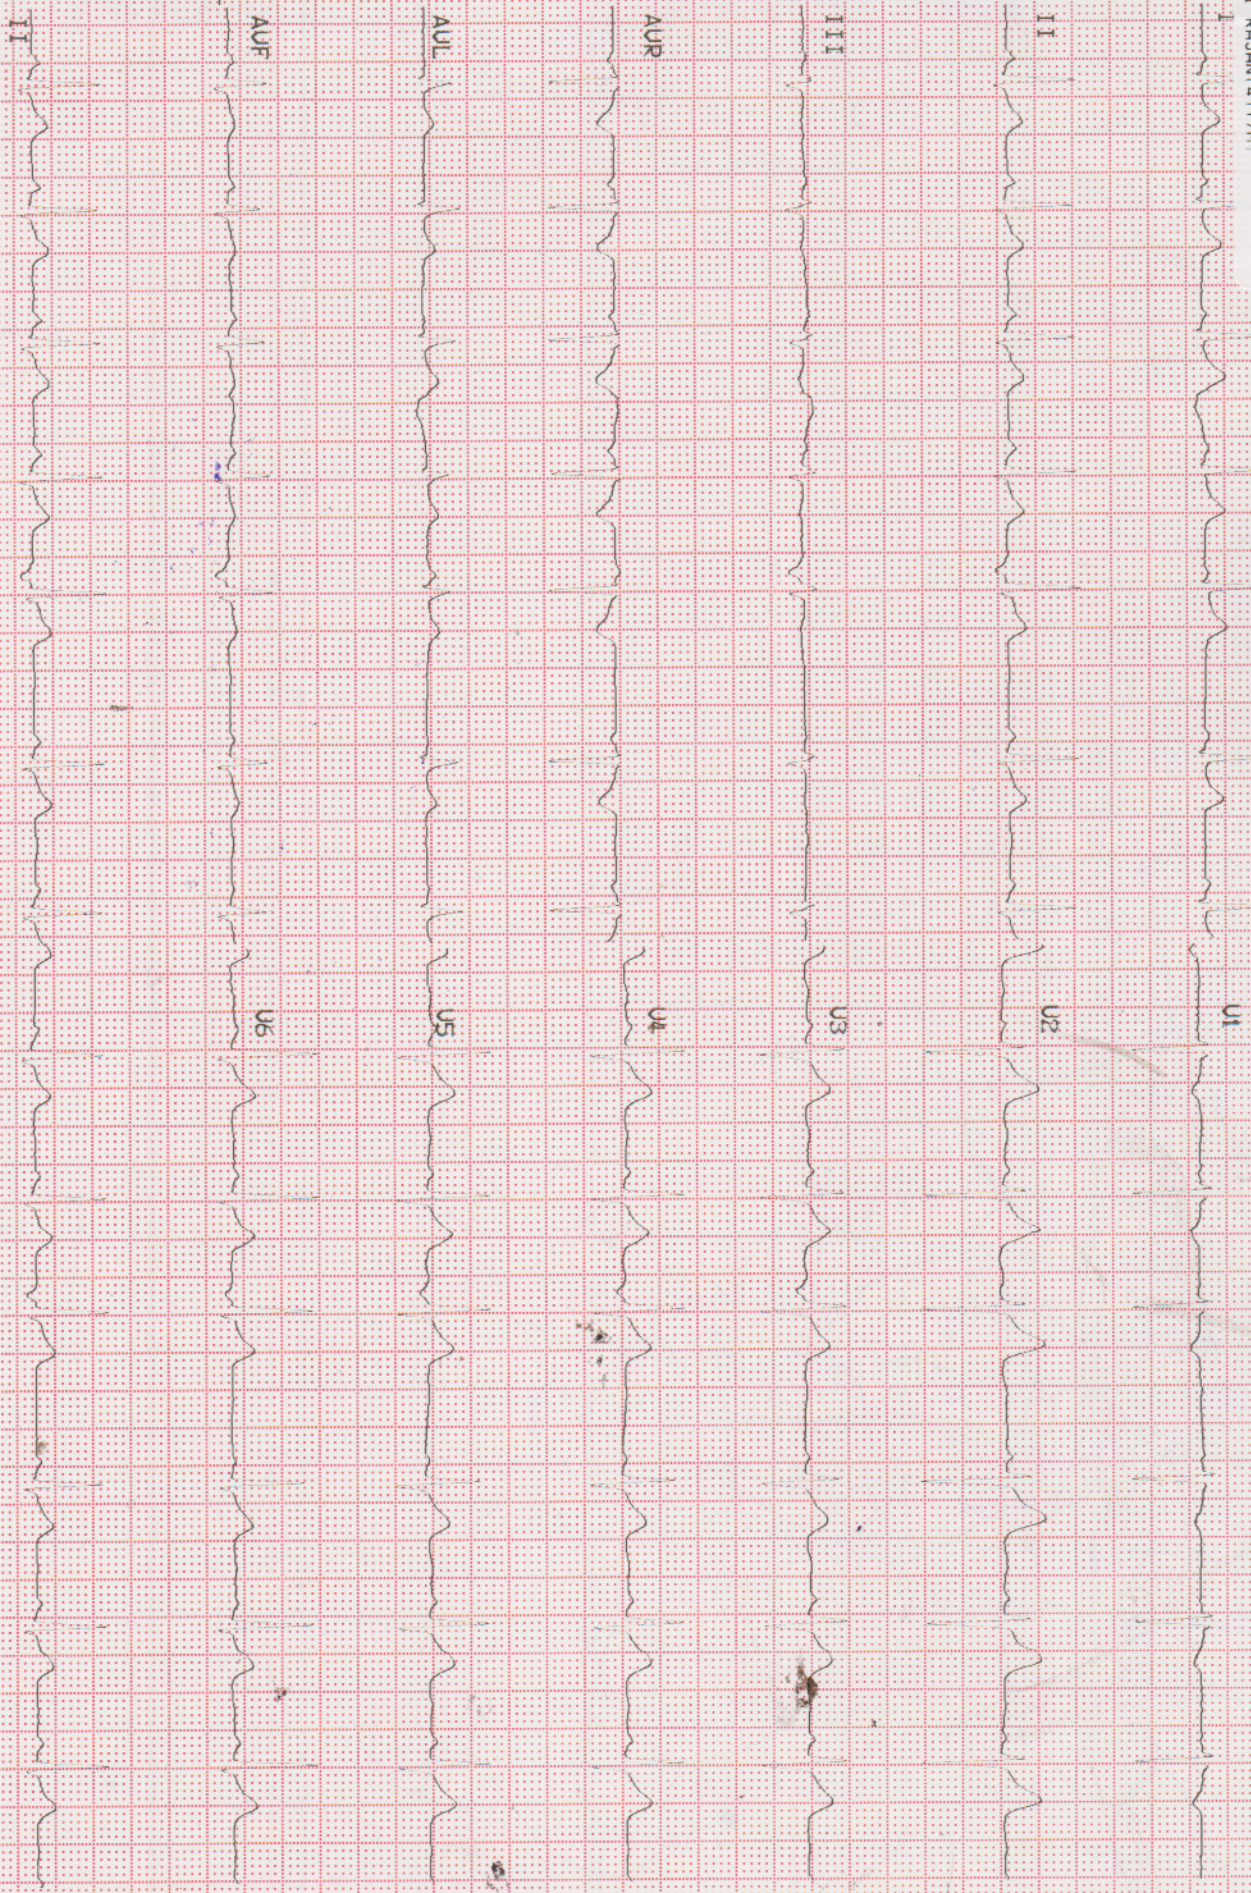

26 Nov 2008 2:00:01.32

25mm/s 10mm/mV ADS 50HZ 0.08-20HZ 6\_FS\_R Automatic U6.2 (1)

9  
2  
1  
9  
5