

आयकर विभाग  
INCOME TAX DEPARTMENT

भारत सरकार  
GOVT. OF INDIA

PRASHANT SANWARIYA  
SHIV HARE SANWARIYA

19/03/1990  
Permanent Account Number  
CNZPS5988M

*Prashant S.*  
Signature

13012010

*Prashant Sanwariya*  
*957162 8525*  
*For Medical Purpose Only*



## SUBURBAN DIAGNOSTICS MALAD(W)

### Patient Details

Date: 12-Feb-22

Time: 10:11:30

Name: PRASHANT SANWARIYA ID: 2204331860

Age: 31 y

Sex: M

Height: 157 cms

Weight: 68 Kgs

### Clinical History:

### Medications:

### Test Details

Protocol: Bruce

Pr.MHR: 189 bpm

THR: 170 (90 % of Pr.MHR) bpm

Total Exec. Time: 9 m 52 s

Max. HR: 172 (91% of Pr.MHR) bpm

Max. Mets: 13.50

Max. BP: 170 / 90 mmHg

Max. BP x HR: 29240 mmHg/min

Min. BP x HR: 5850 mmHg/min

Test Termination Criteria: Target HR attained

### Protocol Details

Stage Name	Stage Time (min : sec)	Mets	Speed (mph)	Grade (%)	Heart Rate (bpm)	Max. BP (mm/Hg)	Max. ST Level (mm)	Max. ST Slope (mV/s)
Supine	0 : 16	1.0	0	0	80	130 / 90	-1.27 aVR	2.48 V3
Standing	0 : 13	1.0	0	0	69	130 / 90	-1.49 aVR	3.18 V3
Hyperventilation	0 : 13	1.0	0	0	65	130 / 90	-0.85 aVR	3.18 V3
1	3 : 0	4.6	1.7	10	111	130 / 90	-1.70 aVR	3.54 V3
2	3 : 0	7.0	2.5	12	132	142 / 90	-1.49 aVR	3.89 V3
3	3 : 0	10.2	3.4	14	158	156 / 90	-2.34 V2	4.95 I
Peak Ex	0 : 52	13.5	4.2	16	172	170 / 90	-4.25 V2	3.89 V2
Recovery(1)	1 : 0	1.8	1	0	151	170 / 90	-2.55 V2	5.66 V3
Recovery(2)	1 : 0	1.0	0	0	123	170 / 90	-2.34 aVR	5.66 V3
Recovery(3)	1 : 0	1.0	0	0	117	170 / 90	-1.70 aVR	5.66 V3
Recovery(4)	1 : 0	1.0	0	0	113	170 / 90	-1.27 aVR	3.89 V3
Recovery(5)	1 : 0	1.0	0	0	112	170 / 90	-1.06 aVR	2.83 V2
Recovery(6)	0 : 5	1.0	0	0	108	170 / 90	-0.85 aVR	2.12 V3

### Interpretation

The patient exercised according to the Bruce protocol for 9 m 52 s achieving a work level of Max. METS : 13.50. Resting heart rate initially 80 bpm, rose to a max. heart rate of 172 (91% of Pr.MHR) bpm. Resting blood Pressure 130 / 90 mmHg, rose to a maximum blood pressure of 170 / 90 mmHg.

Good effort tolerance. Normal chronotropic response. Normal ionotropic response. No anginal/ angina equivalents. No arrhythmia. No significant ST-T changes from baseline.

IMPRESSION: STRESS TEST IS NEGATIVE FOR STRESS INDUCIBLE ISCHEMIA

Disclaimer: Negative test does not rule out Coronary Artery Disease. Positive test is suggestive but not confirmatory of coronary artery disease. Hence clinical correlation is mandatory.

DR. SONALI HONRAO

MD (G.MED)

CONSULTING PHYSICIAN

REG. NO. 2001/04/1882

SUBURBAN DIAGNOSTICS (INDIA) PVT. LTD.

102-104, Bhoomi Castle,

Opp. Goregaon Sports Club,

Link Road, Malad (W), Mumbai - 400 064.

Ref. Doctor: ARCOFEMI

(Summary Report edited by user)

Doctor: DR. SONALI HONRAO

(c) Schiller Healthcare India Pvt. Ltd. V 4.7



# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 130 / 90

Protocol: Bruce

Stage: Supine

Speed: 0 mph


Grade: 0 %

Exec Time : 0 m 0 s

Stage Time : 0 m 16 s

**HR: 80 bpm**

(THR: 170 bpm)

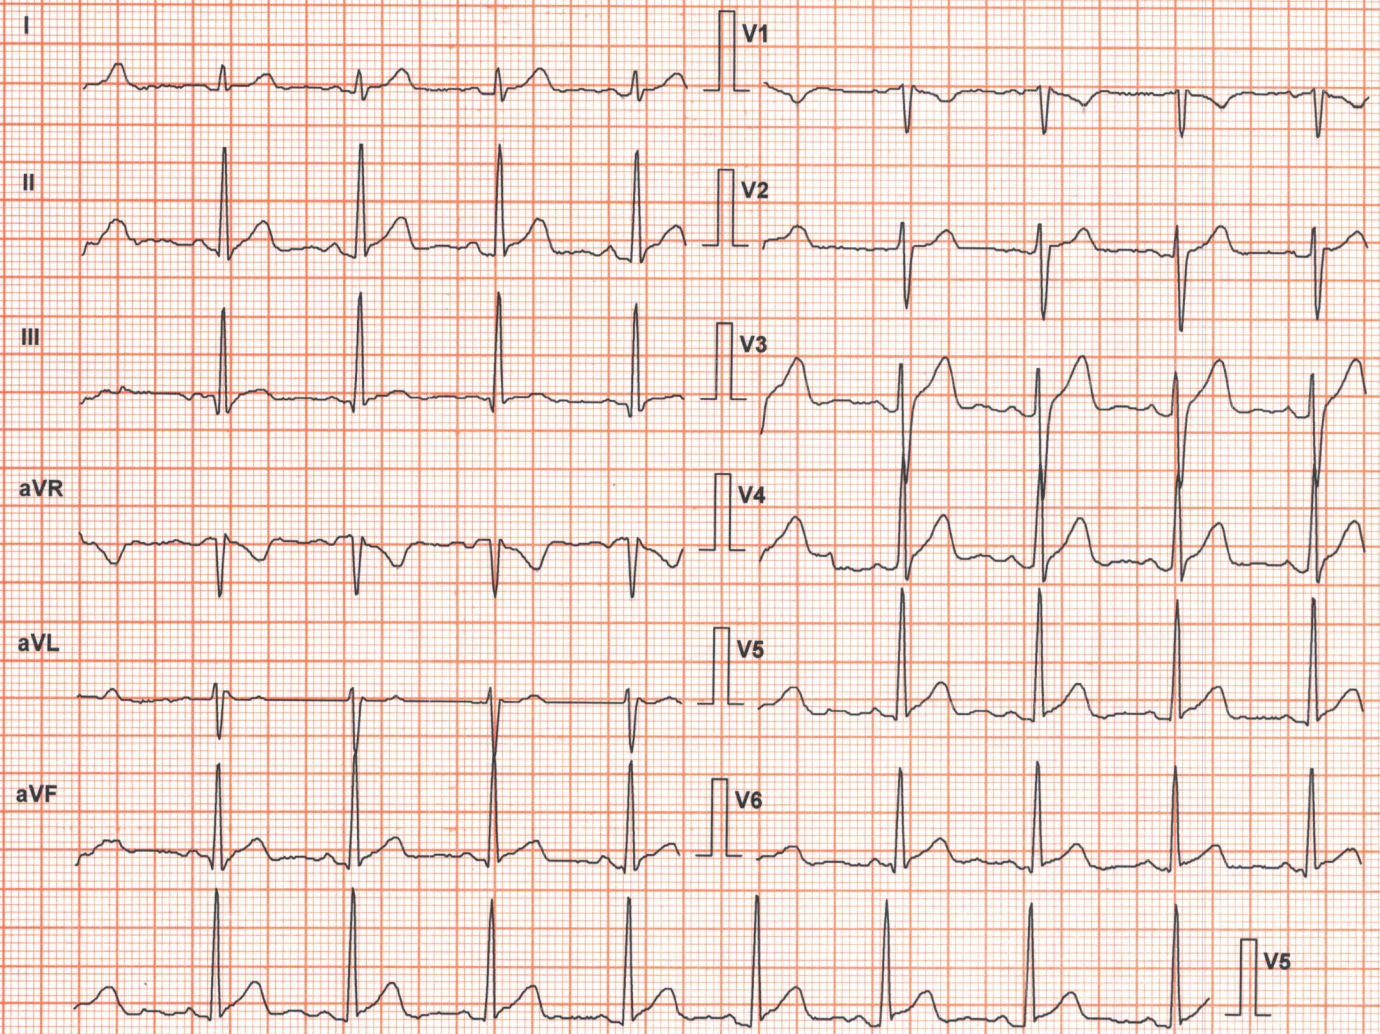

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.8	0.4
II	1.9	0.4
III	0.6	0.4
aVR	-1.3	-0.4
aVL	0.0	0.0
aVF	1.1	0.4
V1	-0.4	0.0
V2	1.1	0.7
V3	3.2	2.5
V4	2.8	1.4
V5	2.1	1.1
V6	1.3	0.7

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 130 / 90

Protocol: Bruce

Stage: Standing

Speed: 0 mph


Grade: 0 %

Exec Time : 0 m 0 s

Stage Time : 0 m 13 s

**HR: 69 bpm**

(THR: 170 bpm)

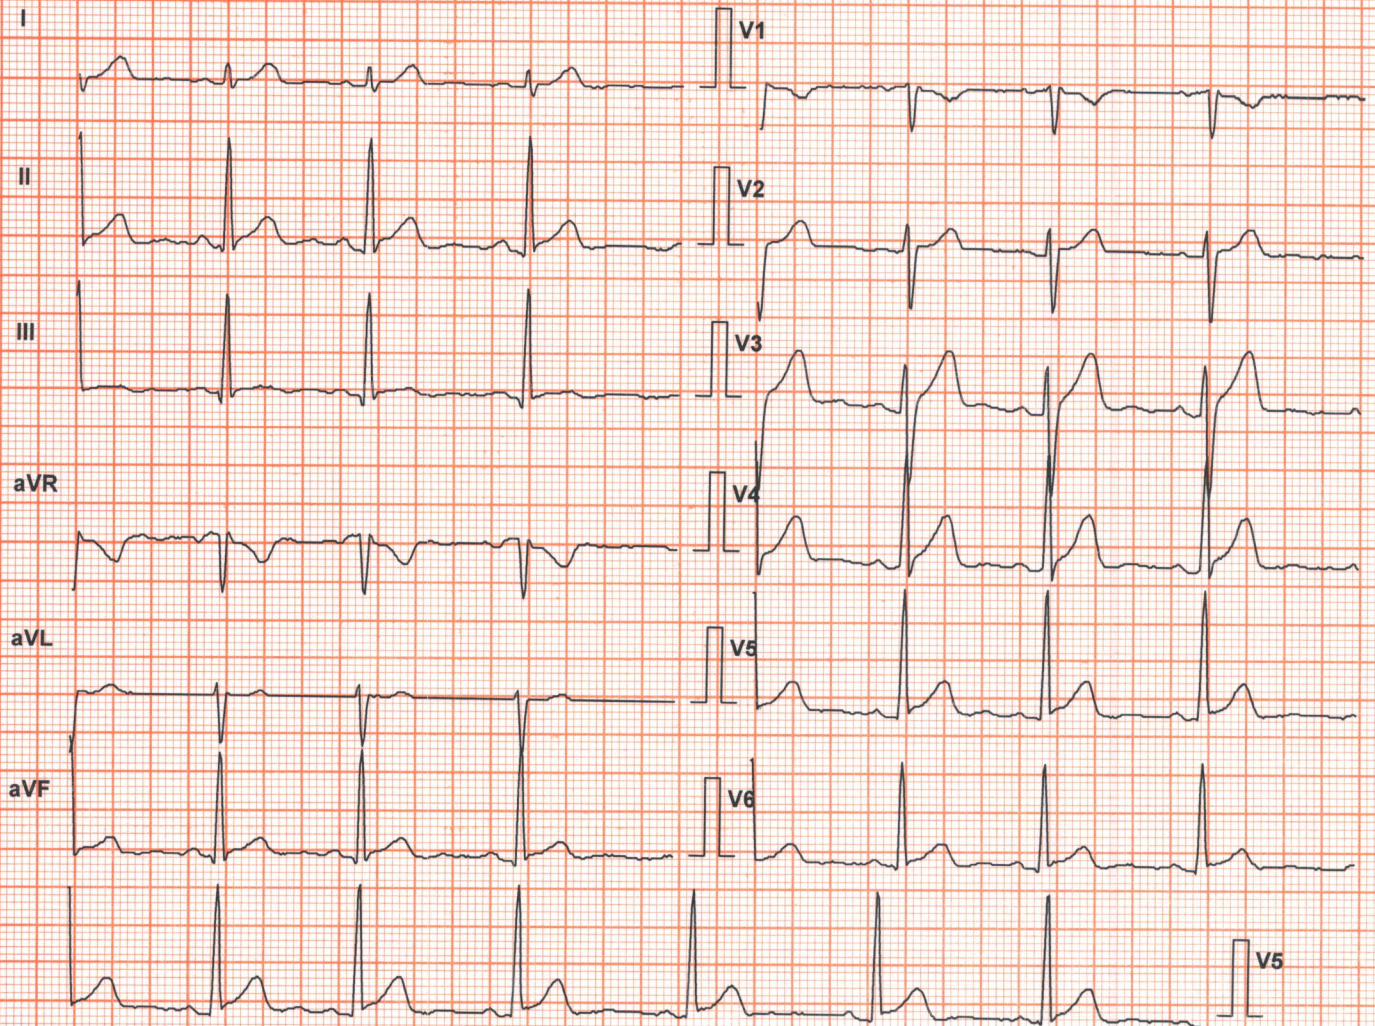

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.6	0.4
II	1.5	0.7
III	0.4	0.0
aVR	-0.8	-0.4
aVL	0.0	0.0
aVF	0.8	0.4
V1	-0.2	0.0
V2	1.1	0.7
V3	3.2	2.5
V4	2.5	1.8
V5	1.5	0.7
V6	0.8	0.4

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 130 / 90

Protocol: Bruce

Stage: Hyperventilation

Speed: 0 mph


Grade: 0 %

Exec Time : 0 m 0 s

Stage Time : 0 m 13 s

**HR: 65 bpm**

(THR: 170 bpm)

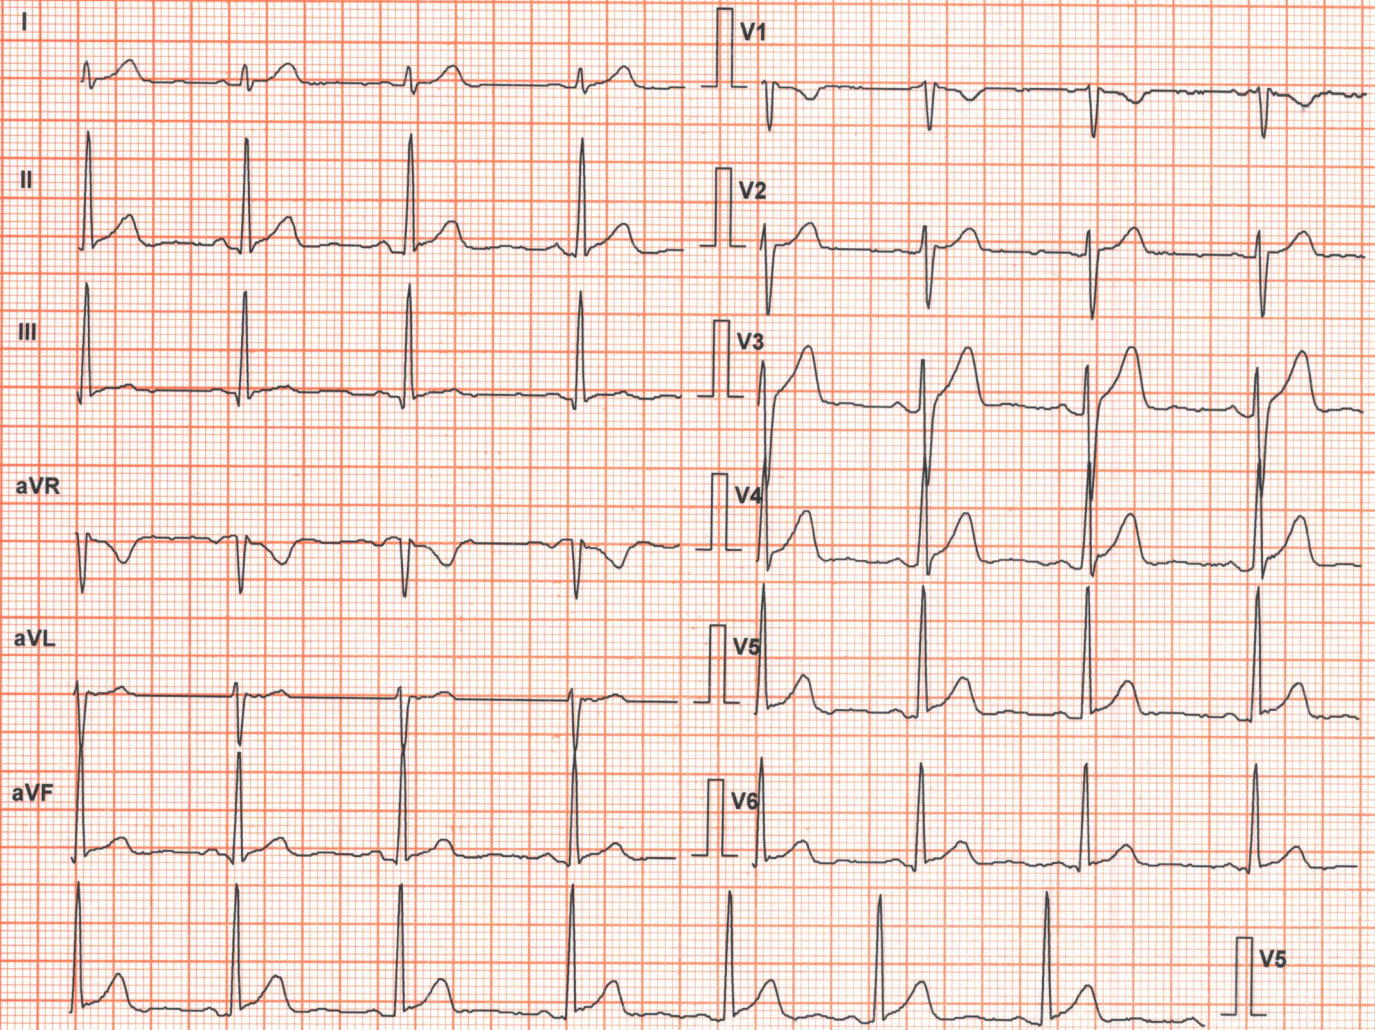

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.6	0.4
II	1.5	0.7
III	0.4	0.0
aVR	-0.8	-0.4
aVL	0.0	0.0
aVF	0.8	0.0
V1	0.0	0.0
V2	1.1	0.7
V3	3.8	3.2
V4	2.8	2.1
V5	1.7	0.7
V6	1.1	0.4

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 130 / 90

Protocol: Bruce

Stage: 1

Speed: 1.7 mph


Grade: 10 %

Exec Time : 3 m 0 s

Stage Time : 3 m 0 s

**HR: 111 bpm**

(THR: 170 bpm)

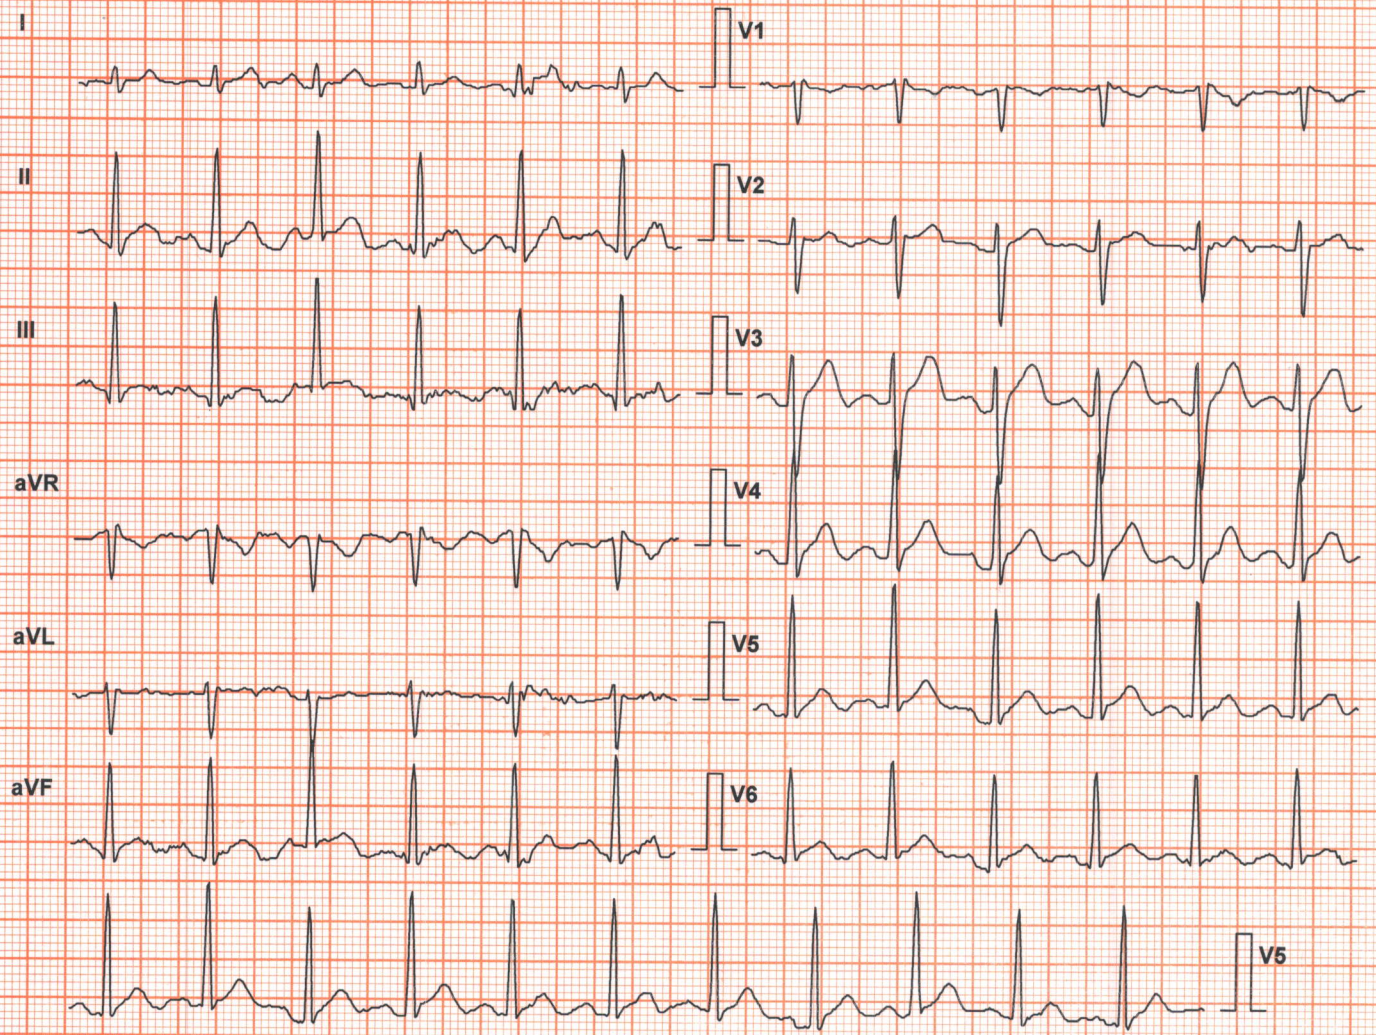

Lead	ST Level (mm)	ST Slope (mV/s)
I	1.1	0.7
aVR	-1.3	-1.1
V1	-0.2	0.0
V4	3.0	2.1
II	1.7	1.8
aVL	0.2	0.0
V2	0.8	1.1
V5	1.7	1.4
III	0.4	0.7
aVF	1.1	1.1
V3	3.8	3.5
V6	1.1	0.7

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 142 / 90

Protocol: Bruce

Stage: 2

Speed: 2.5 mph


Grade: 12 %

Exec Time : 6 m 0 s

Stage Time : 3 m 0 s

**HR: 132 bpm**

(THR: 170 bpm)

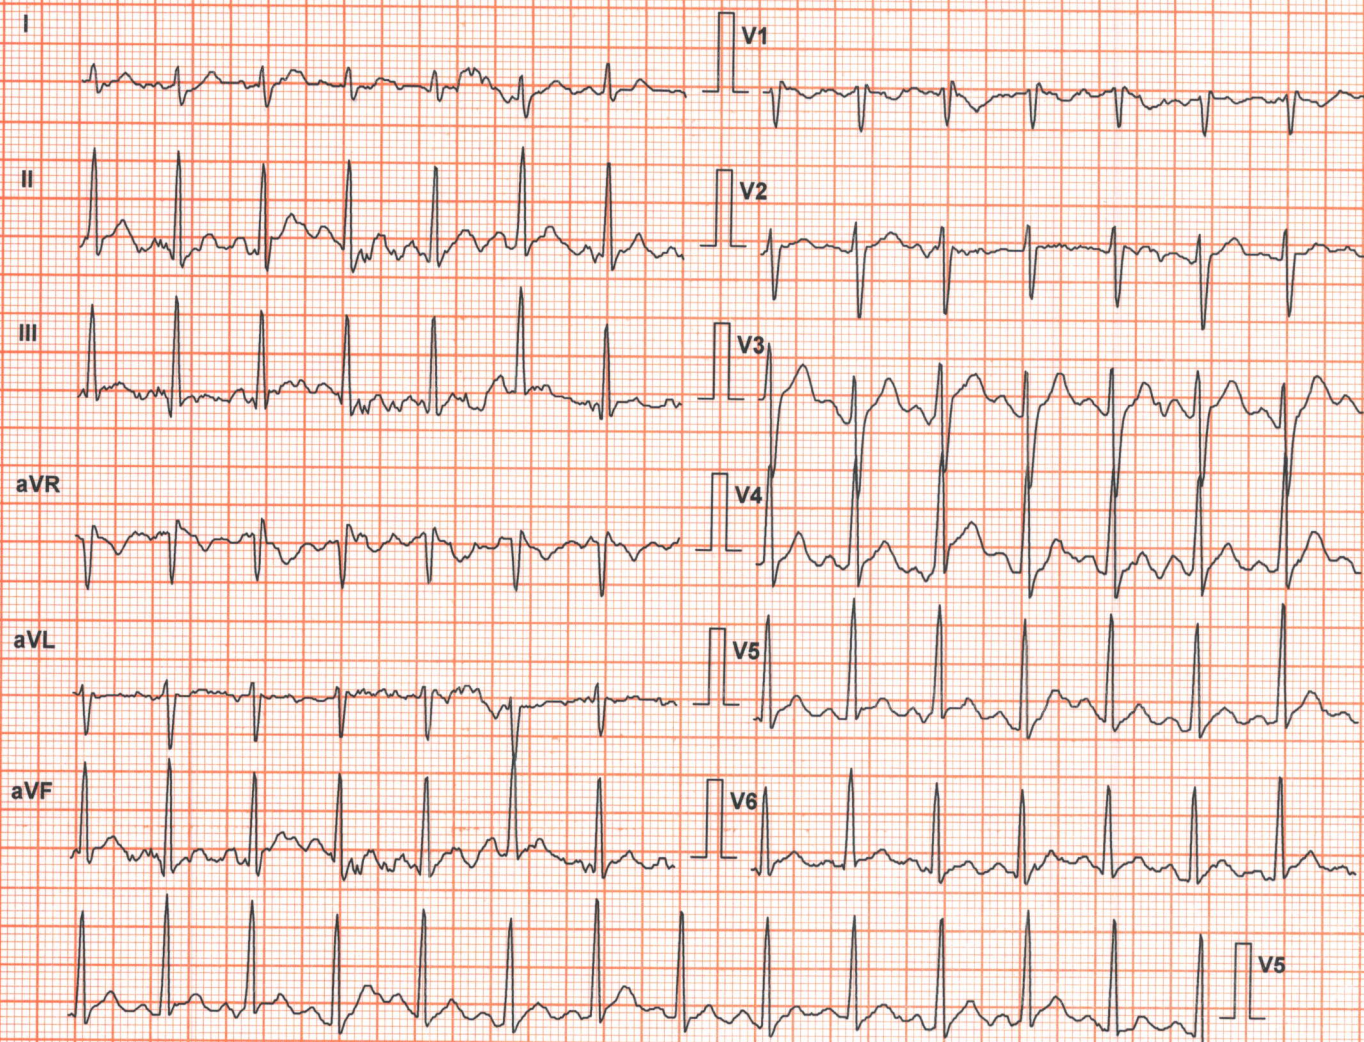

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.8	0.7
aVR	-1.1	-1.1
V1	-0.4	-0.4
V4	2.5	2.1
II	1.5	1.4
aVL	0.0	0.0
V2	0.4	0.7
V5	1.7	1.4
III	0.4	0.7
aVF	0.8	1.1
V3	3.4	3.2
V6	1.1	1.1

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 156 / 90

Protocol: Bruce

Stage: 3

Speed: 3.4 mph


Grade: 14 %

Exec Time : 9 m 0 s

Stage Time : 3 m 0 s

**HR: 158 bpm**

(THR: 170 bpm)

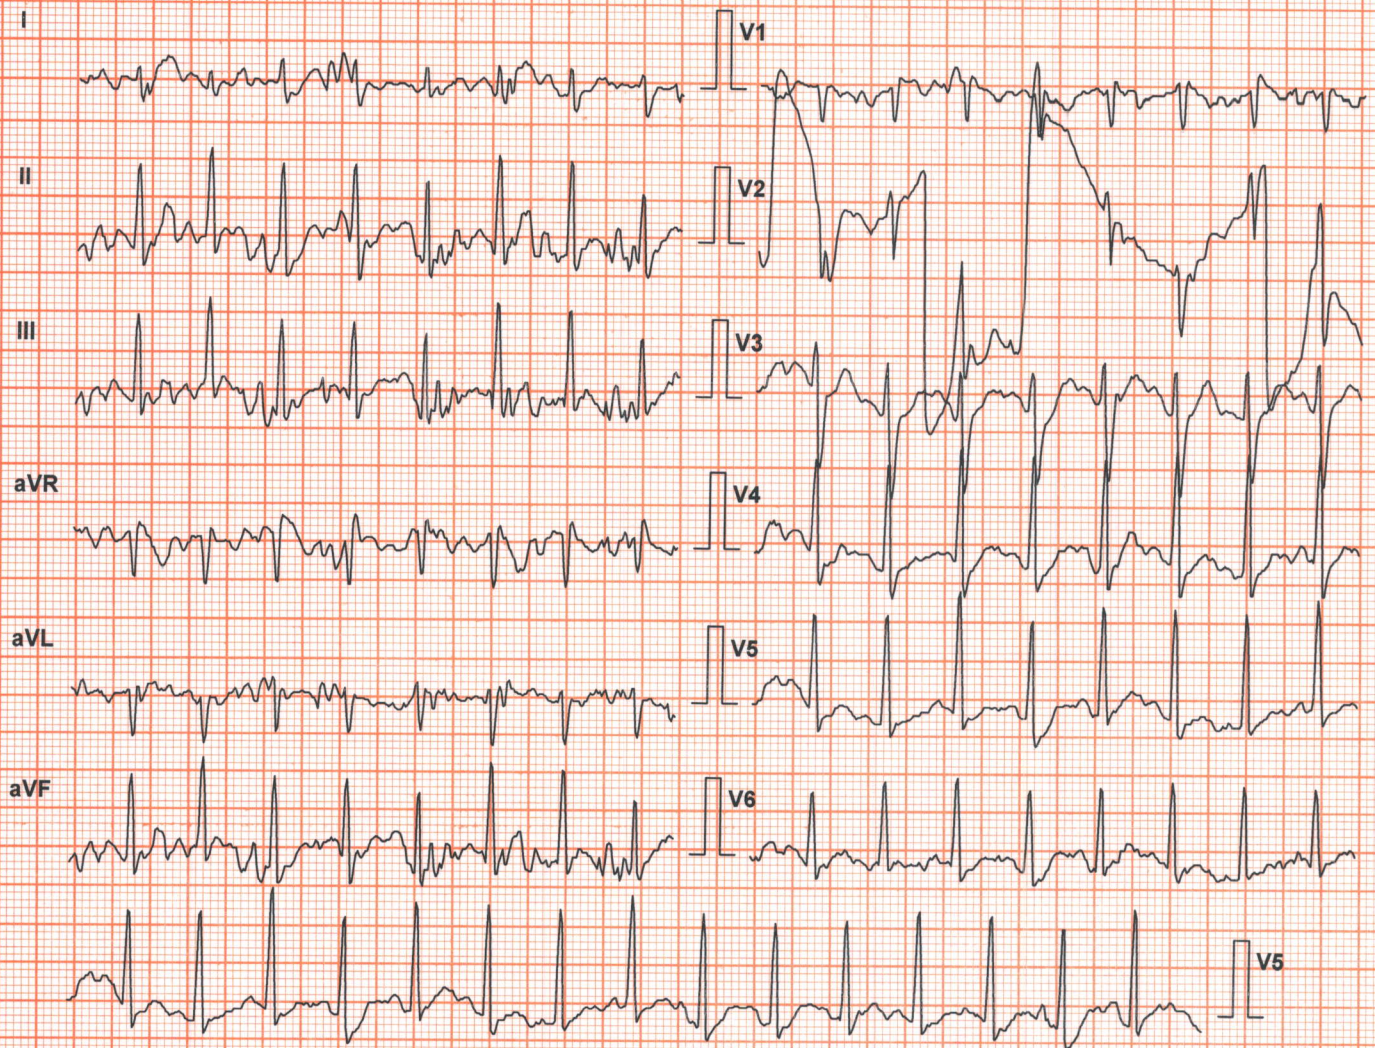

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.6	1.8
aVR	-0.6	-1.8
V1	-0.4	-0.7
V4	1.9	3.5
II	0.8	1.8
aVL	0.4	0.7
V2	1.3	2.5
V5	1.1	2.5
III	0.2	0.4
aVF	0.4	1.1
V3	2.5	3.9
V6	0.6	1.8

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 170 / 90

Protocol: Bruce

Stage: Peak Ex

Speed: 4.2 mph


Grade: 16 %

Exec Time : 9 m 52 s

Stage Time : 0 m 52 s

**HR: 172 bpm**

(THR: 170 bpm)

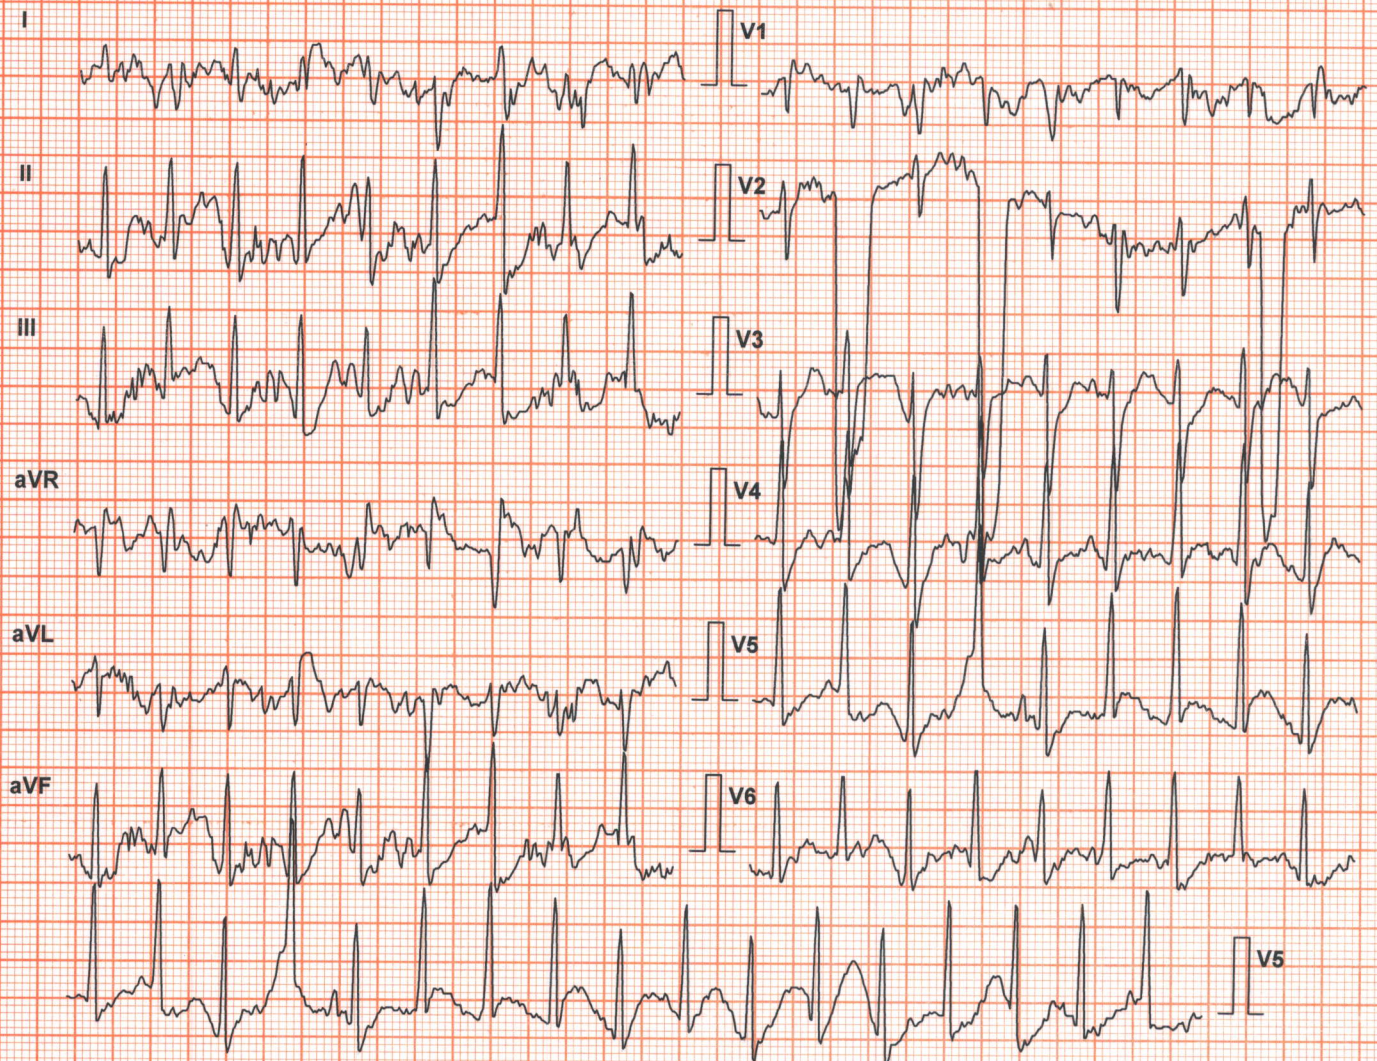

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.0	0.0
aVR	-0.4	-0.7
V1	-0.6	-1.1
V4	0.6	2.8
II	0.6	1.8
aVL	0.0	-0.7
V2	0.0	3.9
V5	-0.2	1.8
III	0.2	1.4
aVF	0.4	1.8
V3	1.1	1.8
V6	0.0	1.4

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 170 / 90

Protocol: Bruce

Stage: Recovery(1)

Speed: 0 mph


Grade: 0 %

Exec Time : 9 m 52 s

Stage Time : 1 m 0 s

**HR: 151 bpm**

(THR: 170 bpm)

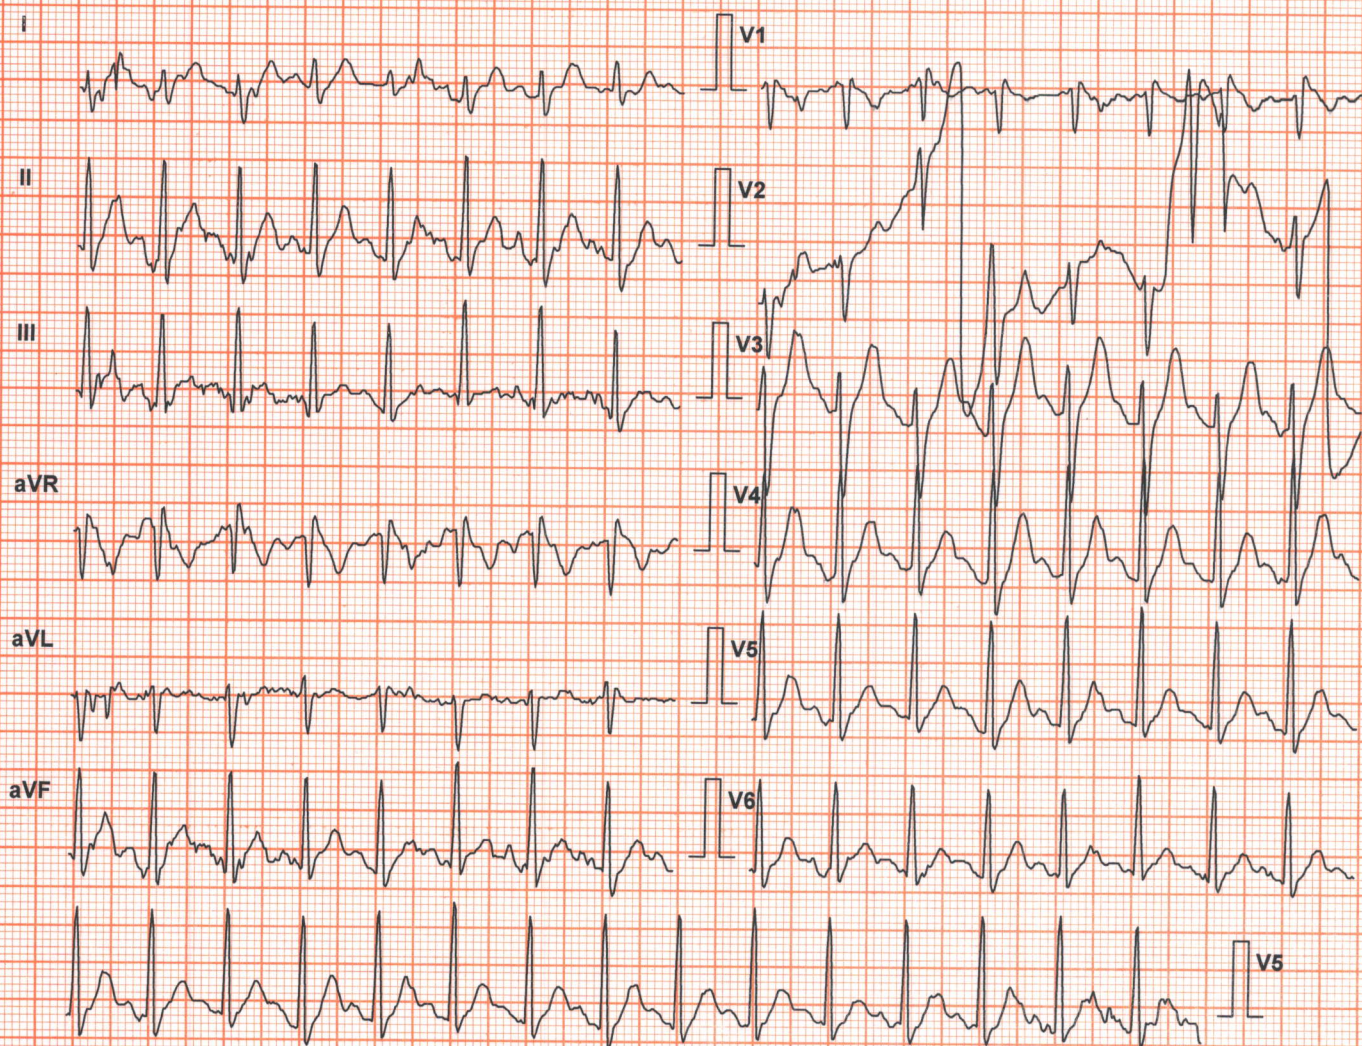

Lead	ST Level (mm)	ST Slope (mV/s)
I	1.5	2.1
aVR	-1.9	-2.8
V1	-0.8	-1.1
V4	4.5	5.7
II	2.5	3.9
aVL	0.2	0.4
V2	3.0	1.8
V5	3.0	4.2
III	0.6	1.1
aVF	1.5	2.5
V3	5.7	5.7
V6	1.7	2.5

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 170 / 90

Protocol: Bruce

Stage: Recovery(2)

Speed: 0 mph


Grade: 0 %

Exec Time : 9 m 52 s

Stage Time : 1 m 0 s

**HR: 123 bpm**

(THR: 170 bpm)

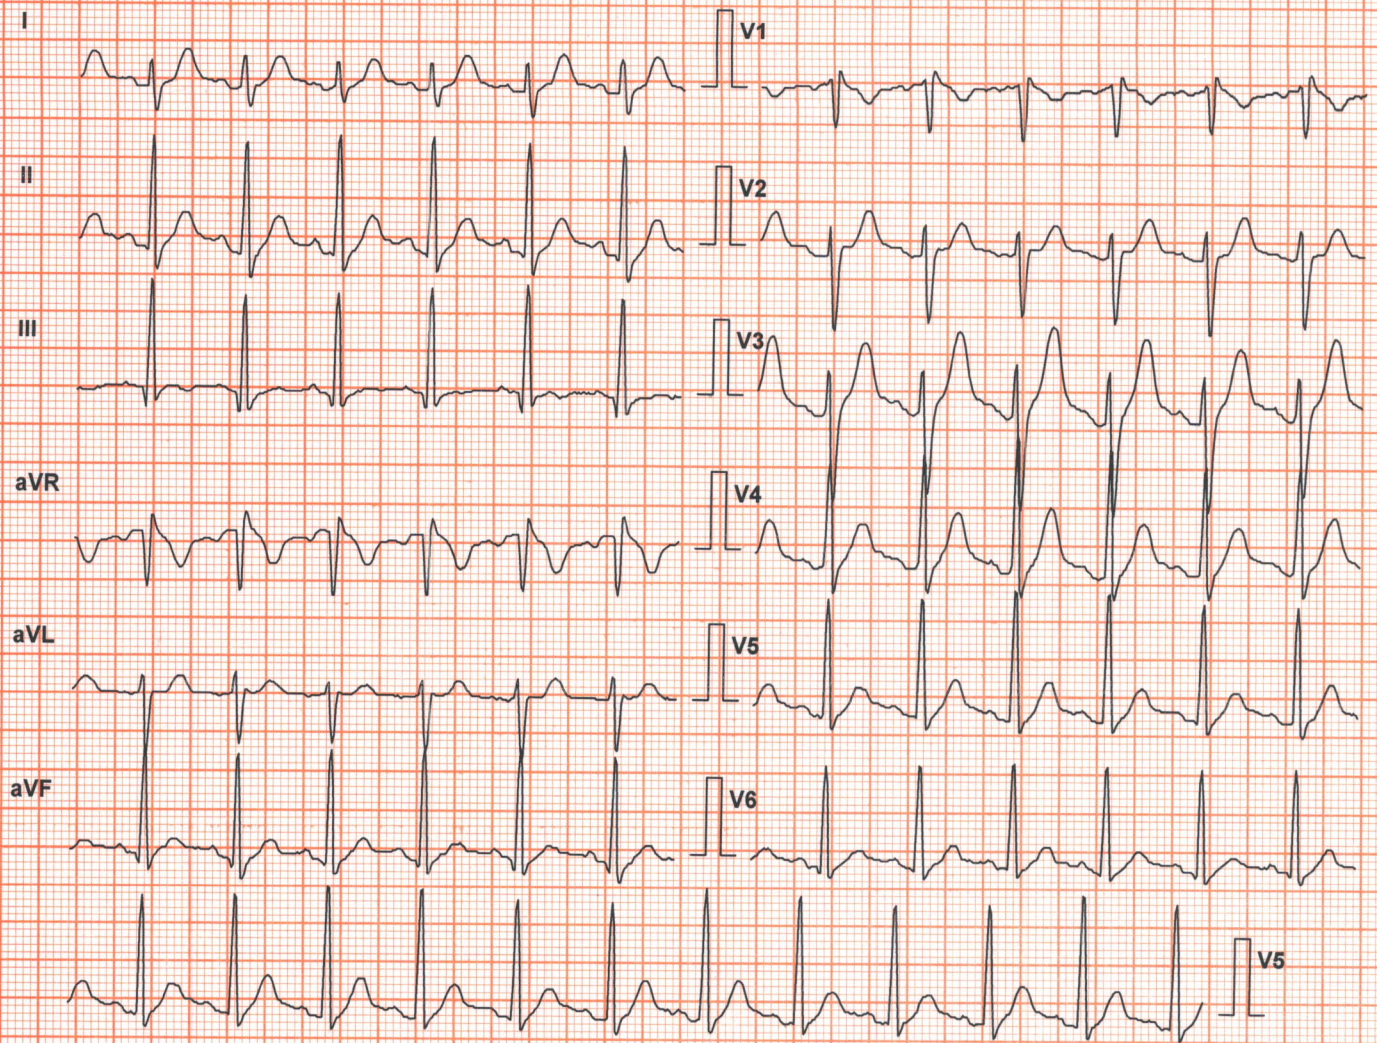

Lead	ST Level (mm)	ST Slope (mV/s)
I	1.5	2.1
II	1.7	2.8
III	0.0	0.7
aVR	-1.7	-2.1
aVL	0.4	0.7
aVF	0.8	1.8
V1	-0.6	-1.1
V2	1.7	1.8
V3	5.3	5.3
V4	3.6	4.2
V5	1.7	2.5
V6	1.1	1.4

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filtr: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 170 / 90

Protocol: Bruce

Stage: Recovery(3)

Speed: 0 mph


Grade: 0 %

Exec Time : 9 m 52 s

Stage Time : 1 m 0 s

**HR: 117 bpm**

(THR: 170 bpm)

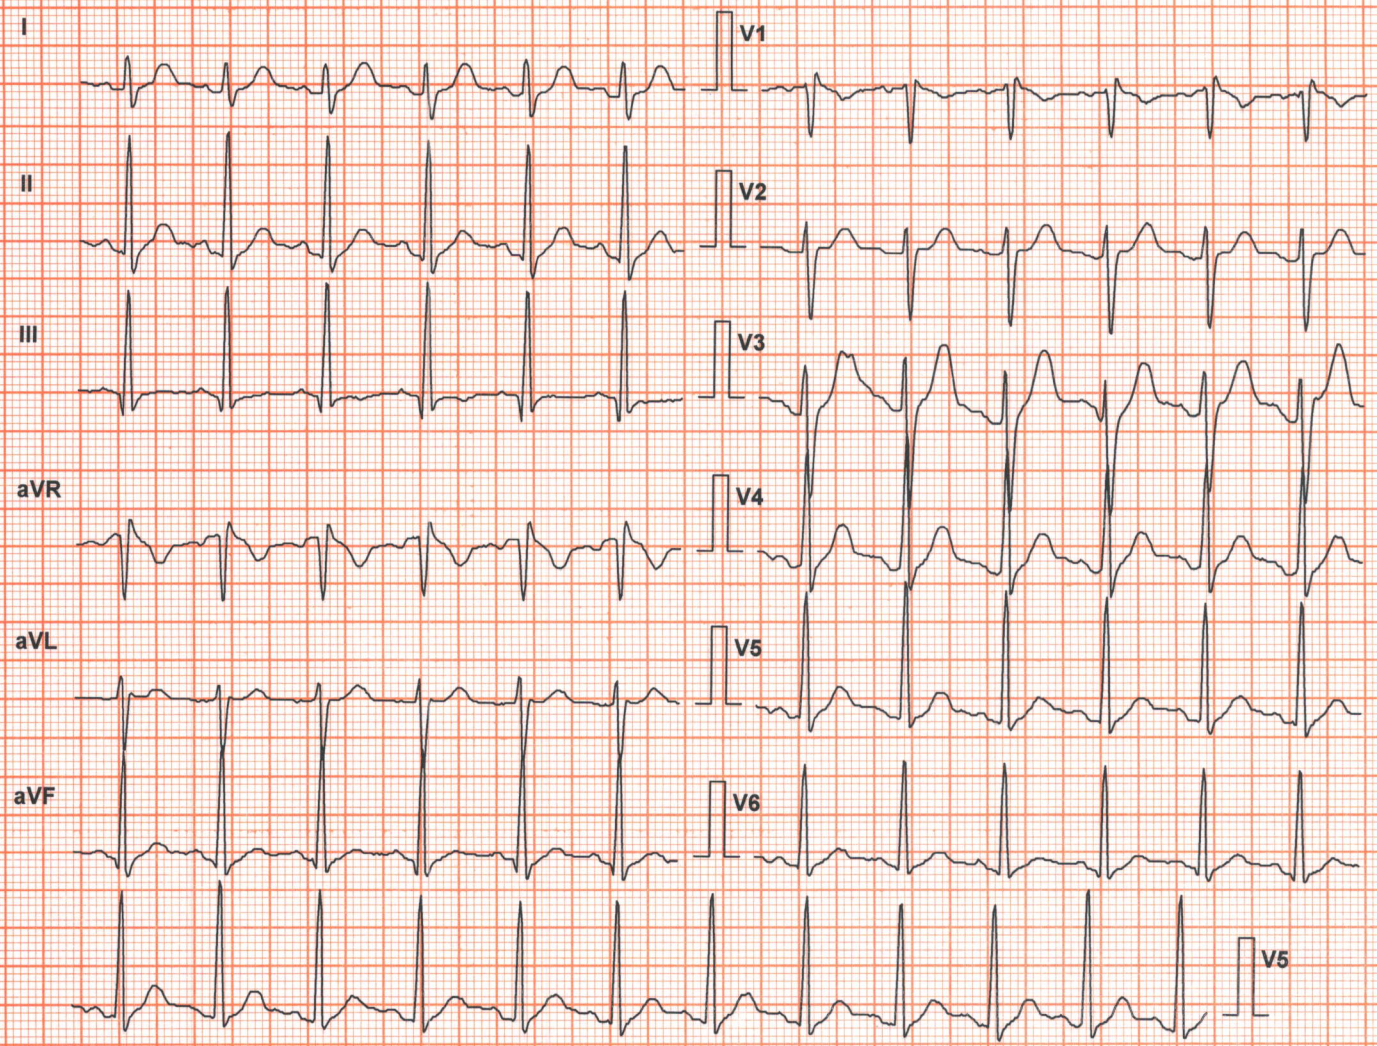

Lead	ST Level (mm)	ST Slope (mV/s)
I	1.1	1.1
II	1.3	2.1
III	0.0	0.7
aVR	-1.1	-1.1
aVL	0.2	0.4
aVF	0.8	1.4
V1	-0.2	-0.4
V2	1.1	0.7
V3	3.6	3.9
V4	2.1	2.5
V5	1.3	1.8
V6	0.8	1.4

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 170 / 90

Protocol: Bruce

Stage: Recovery(4)

Speed: 0 mph


Grade: 0 %

Exec Time : 9 m 52 s

Stage Time : 1 m 0 s

**HR: 113 bpm**

(THR: 170 bpm)

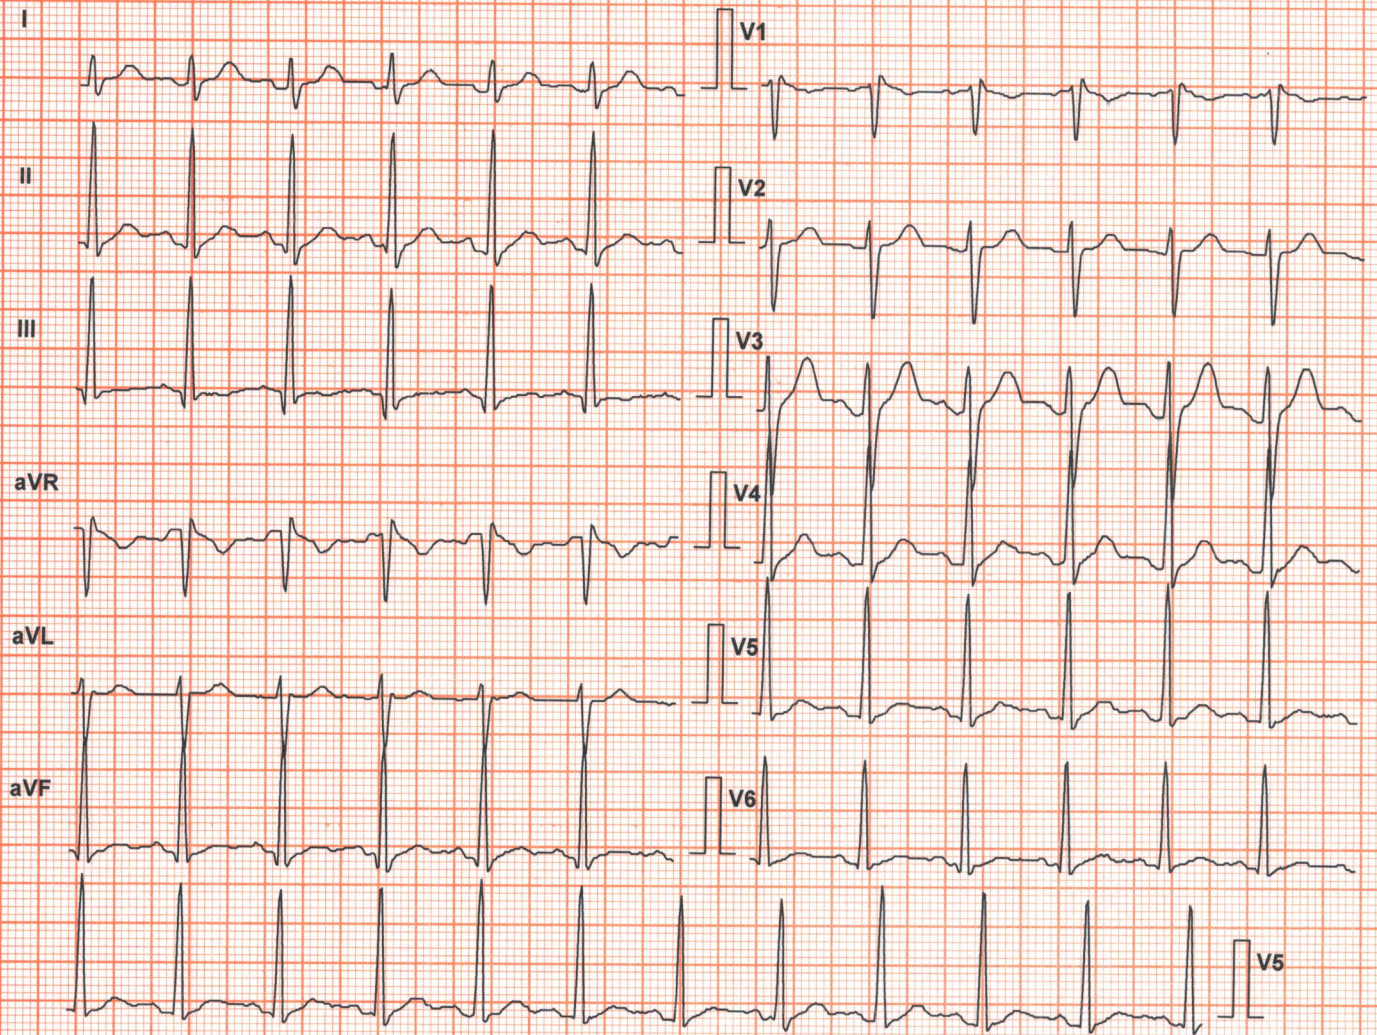

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.6	0.4
II	1.1	1.8
III	0.0	0.7
aVR	-0.8	-1.1
aVL	0.2	0.4
aVF	0.4	1.1
V1	-0.2	-0.4
V2	0.6	0.4
V3	2.5	2.1
V4	1.5	1.4
V5	1.1	1.4
V6	0.4	0.7

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms





# SUBURBAN DIAGNOSTICS MALAD(W)

**PRASHANT SANWARIYA (31 M)**

ID: 2204331860

Date: 12-Feb-22

B.P: 170 / 90

Protocol: Bruce

Stage: Recovery(5)

Speed: 0 mph


Grade: 0 %

Exec Time : 9 m 52 s

Stage Time : 1 m 0 s

**HR: 112 bpm**

(THR: 170 bpm)

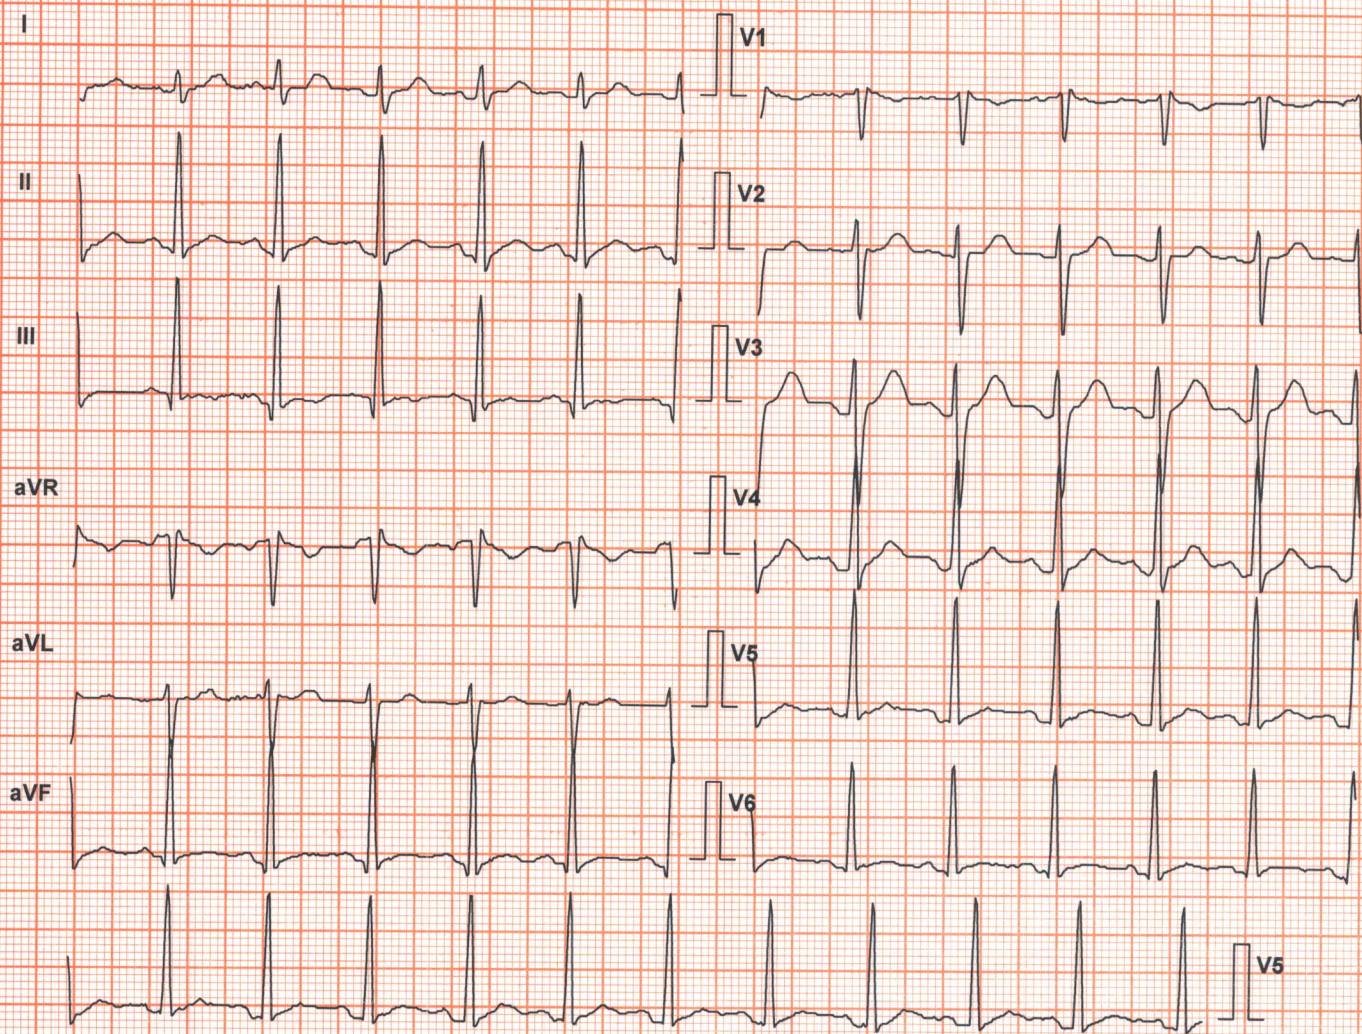

Lead	ST Level (mm)	ST Slope (mV/s)
I	0.4	0.0
II	1.1	1.4
III	0.2	0.4
aVR	-0.8	-0.7
aVL	0.0	0.0
aVF	0.8	1.1
V1	-0.2	-0.4
V2	0.4	0.4
V3	2.1	1.4
V4	1.5	1.1
V5	1.3	1.1
V6	0.8	0.7

Chart Speed: 25 mm/sec

Filter: 35 Hz

Mains Filt: ON

Amp: 10 mm

Schiller Spandan V 4.7

Iso = R - 60 ms J = R + 60 ms

Post J = J + 60 ms

