



Date: 14 - 09 - 2024

METs : 1.1 HR : 77 Target HR : 48% of 162 BP : 0/0

ExTime : 00:00 1.7 mph 10.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz



Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Date: 14 - 09 - 2024

METs : 4.7 HR : 89 Target HR : 55% of 162 BP : 135/86

ExTime : 03:00 1.7 mph 10.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz




Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Date: 14 - 09 - 2024

METs : 7.1 HR : 95 Target HR : 59% of 162 BP : 140/90

ExTime : 06:00 2.5 mph 12.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz

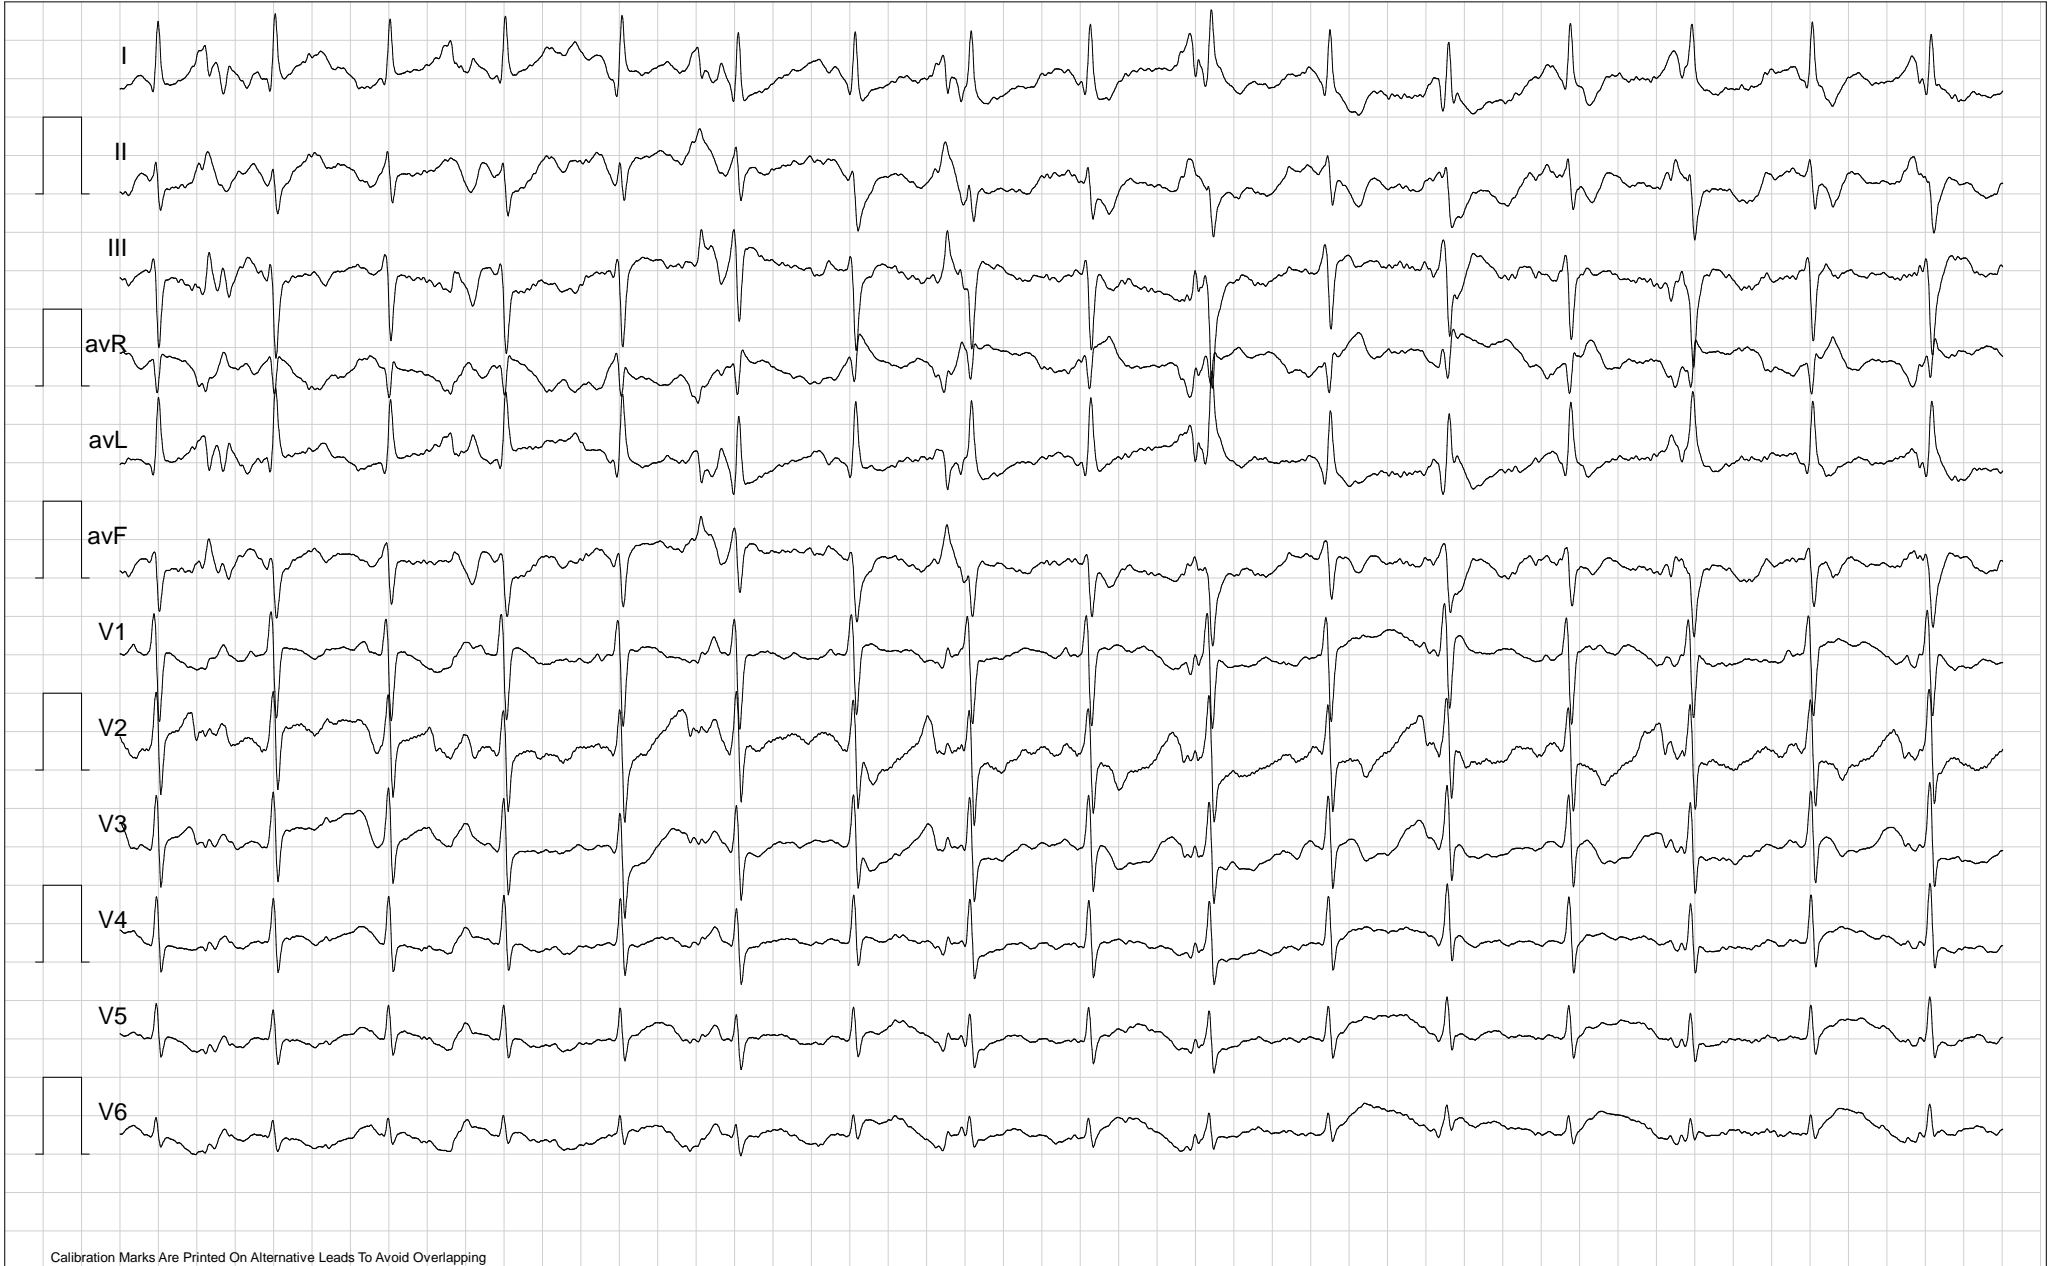


Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Date: 14 - 09 - 2024

METs : 10.2 HR : 115 Target HR : 71% of 162 BP : 145/95

ExTime : 09:00 3.4 mph 14.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz

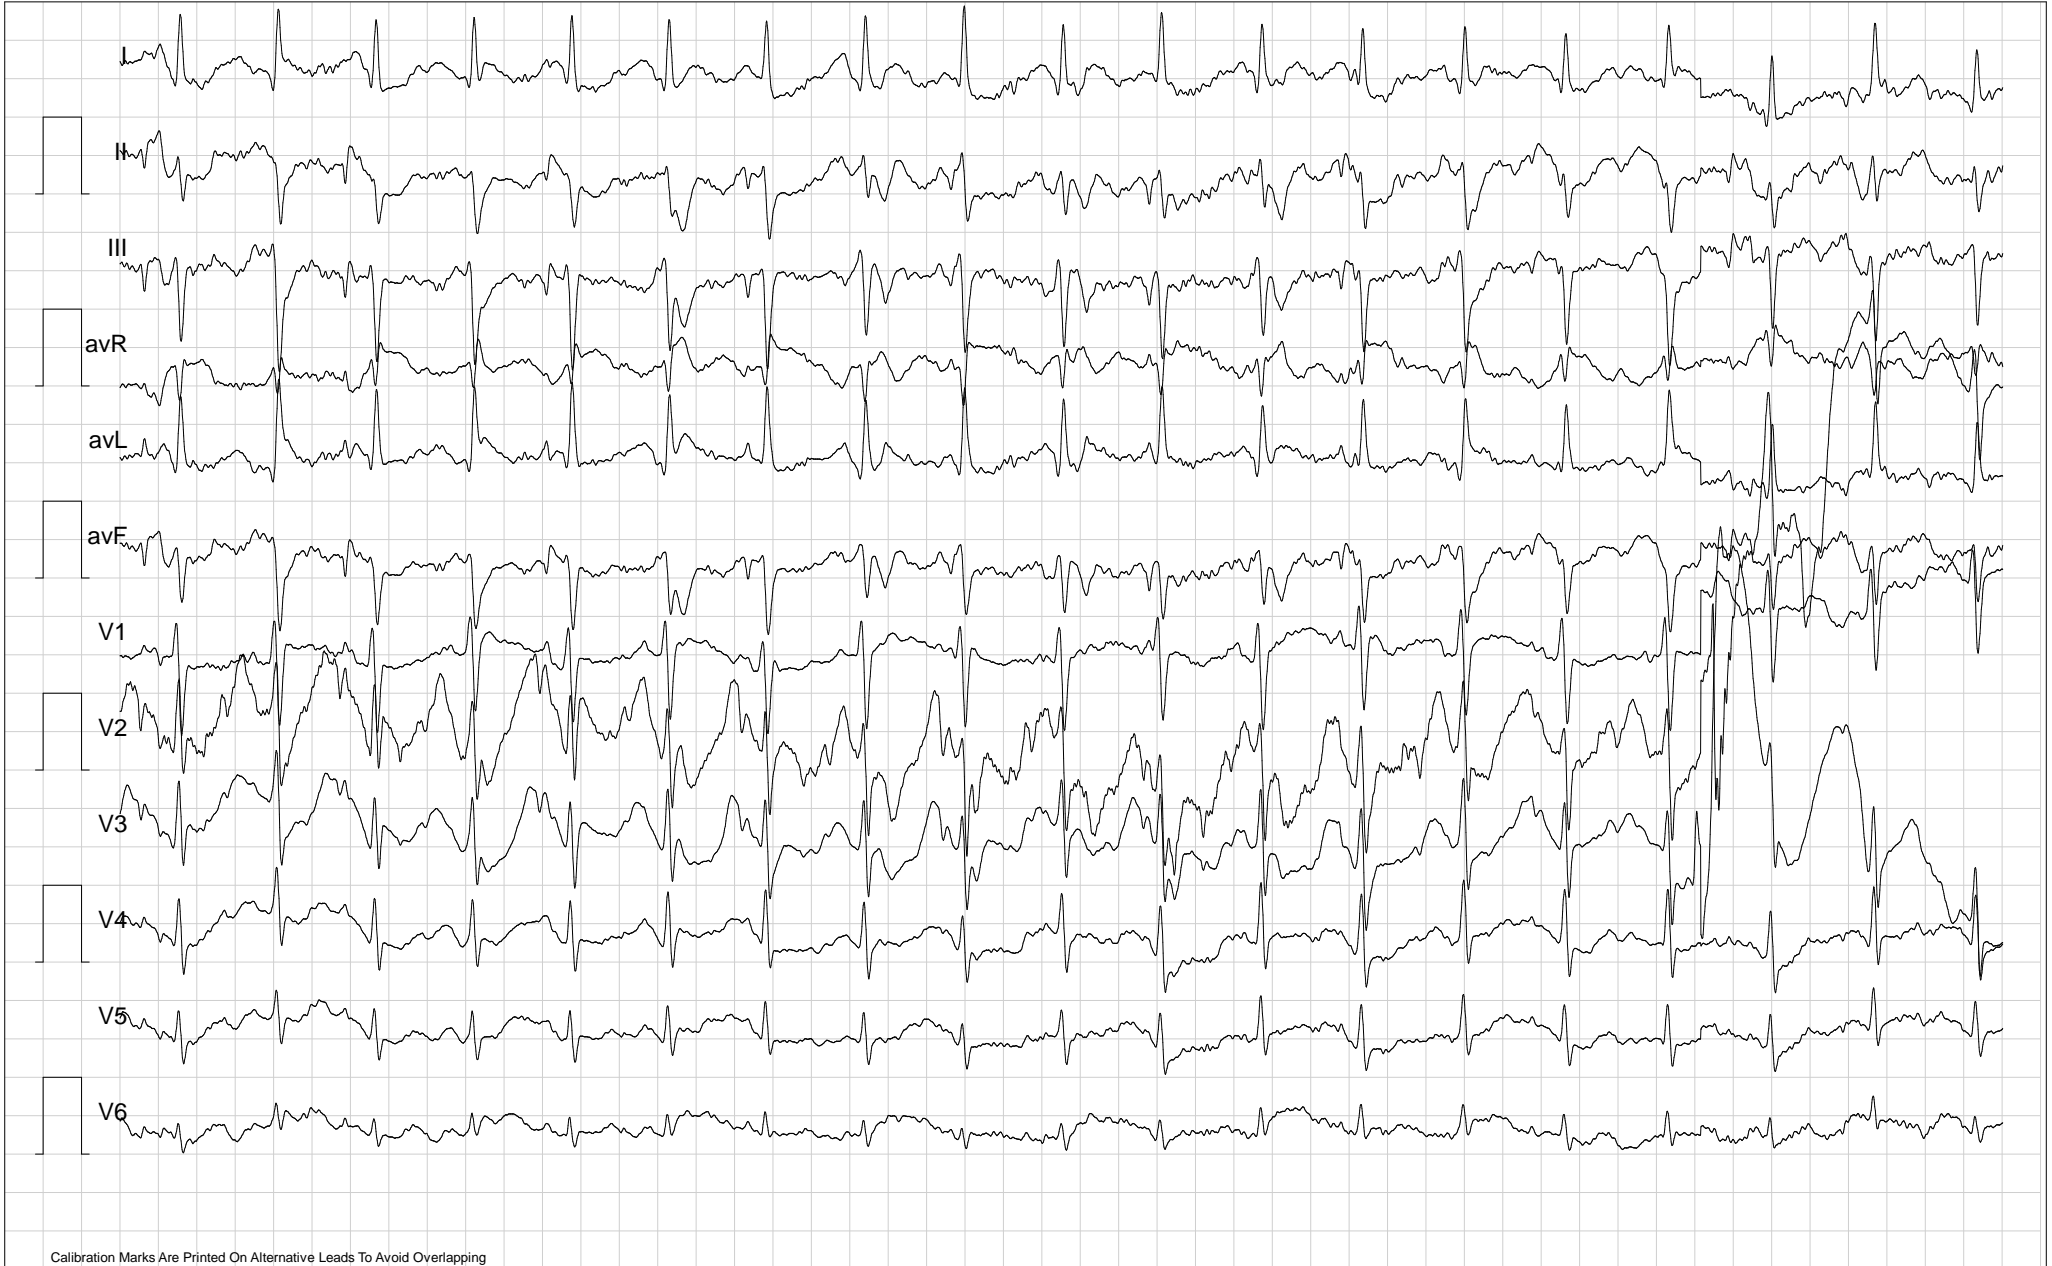


Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Date: 14 - 09 - 2024

METs : 13.5 HR : 128 Target HR : 79% of 162 BP : 155/100

ExTime : 12:00 4.2 mph 16.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz

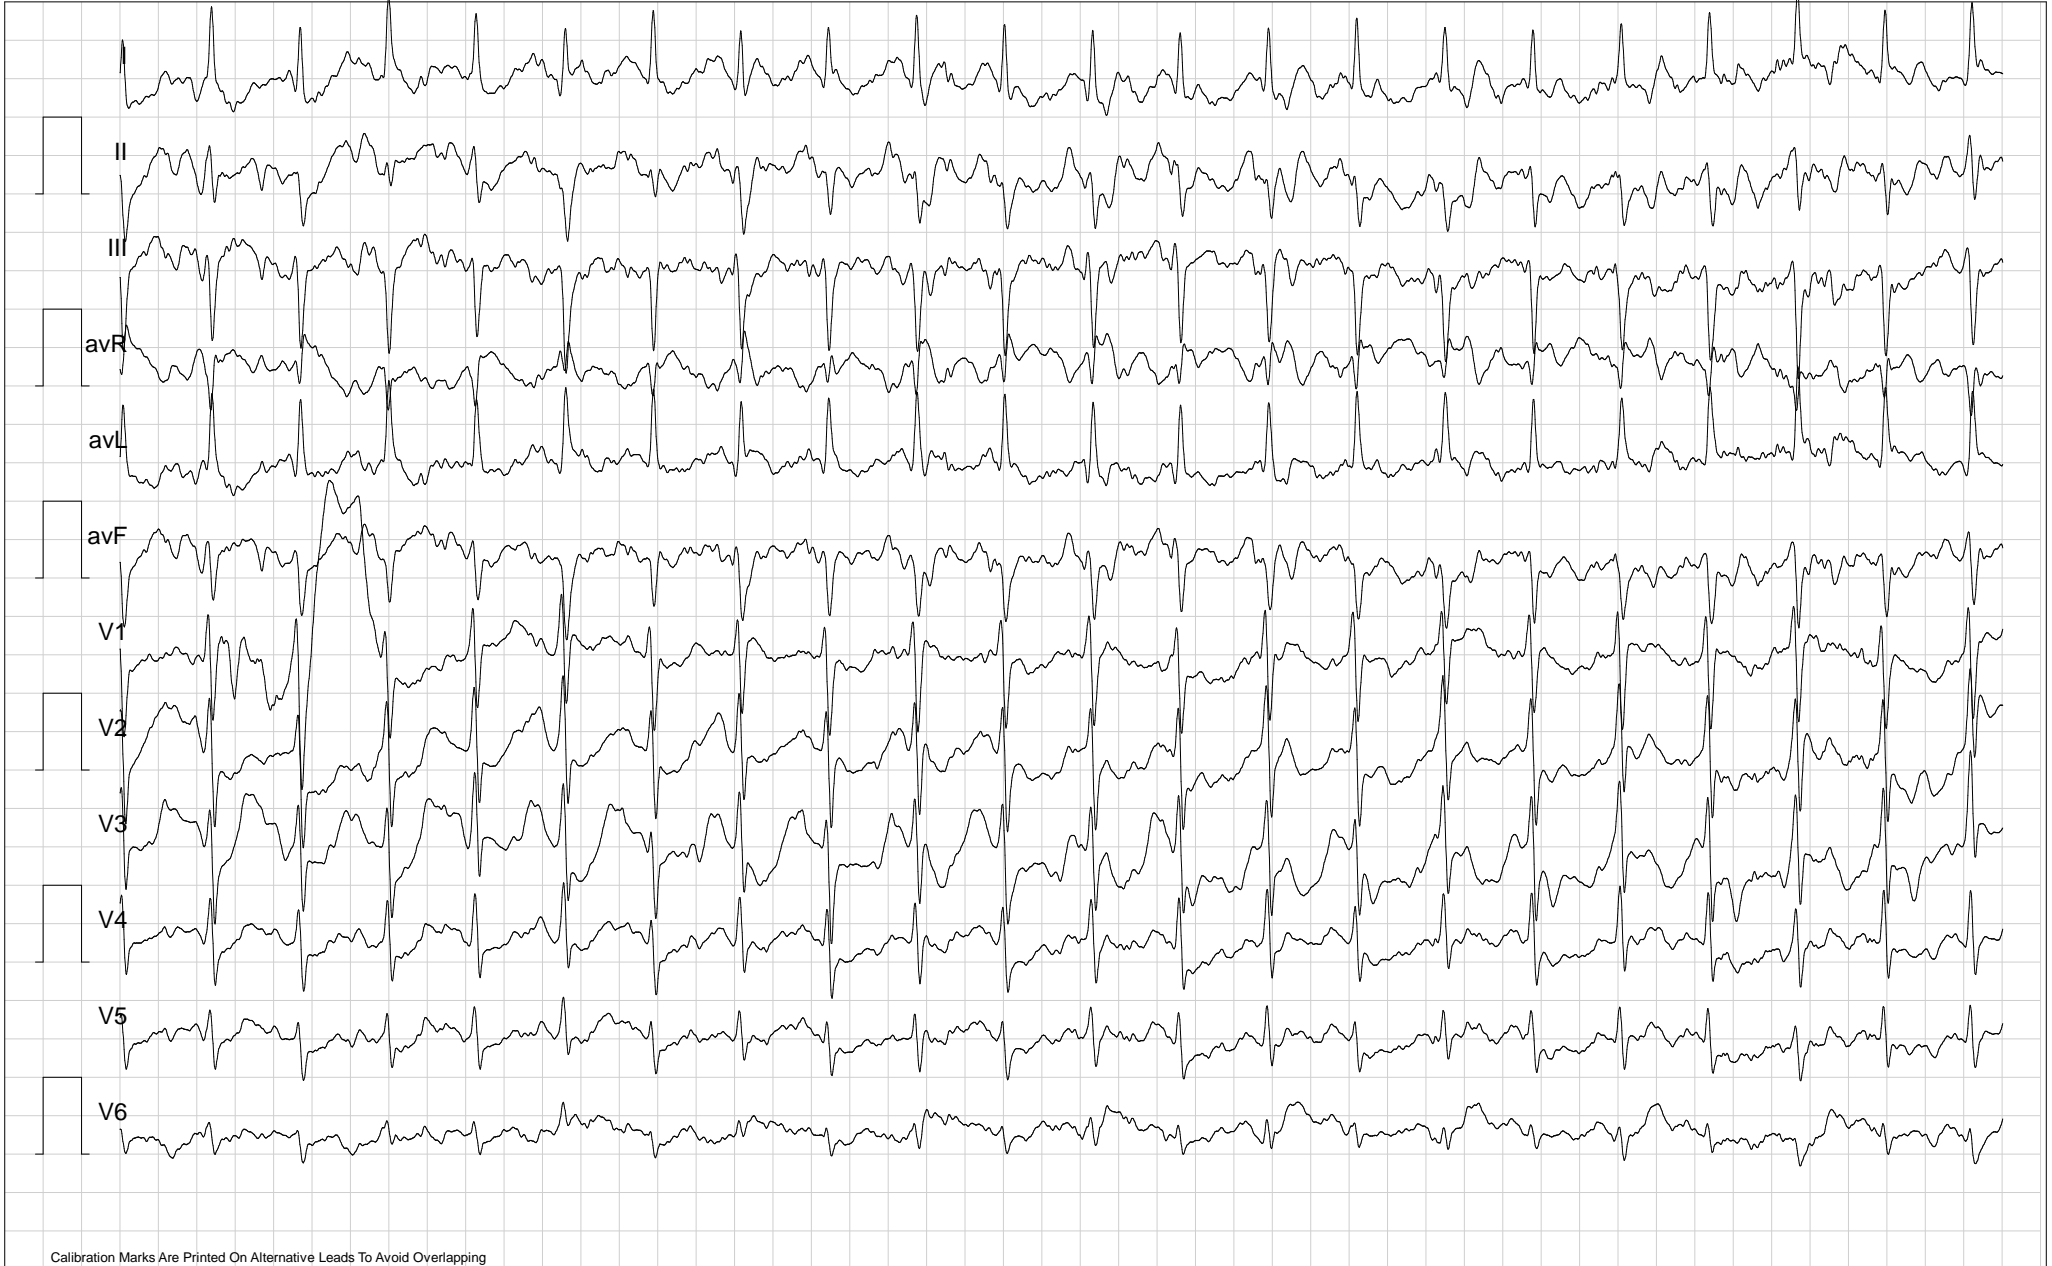

Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping

Date: 14 - 09 - 2024

METs : 13.8 HR : 136 Target HR : 84% of 162 BP : 155/100

ExTime : 12:35 5.0 mph 18.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz




Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Date: 14 - 09 - 2024

METs : 7.5 HR : 119 Target HR : 73% of 162 BP : 160/105

ExTime : 12:35 1.1 mph 0.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz

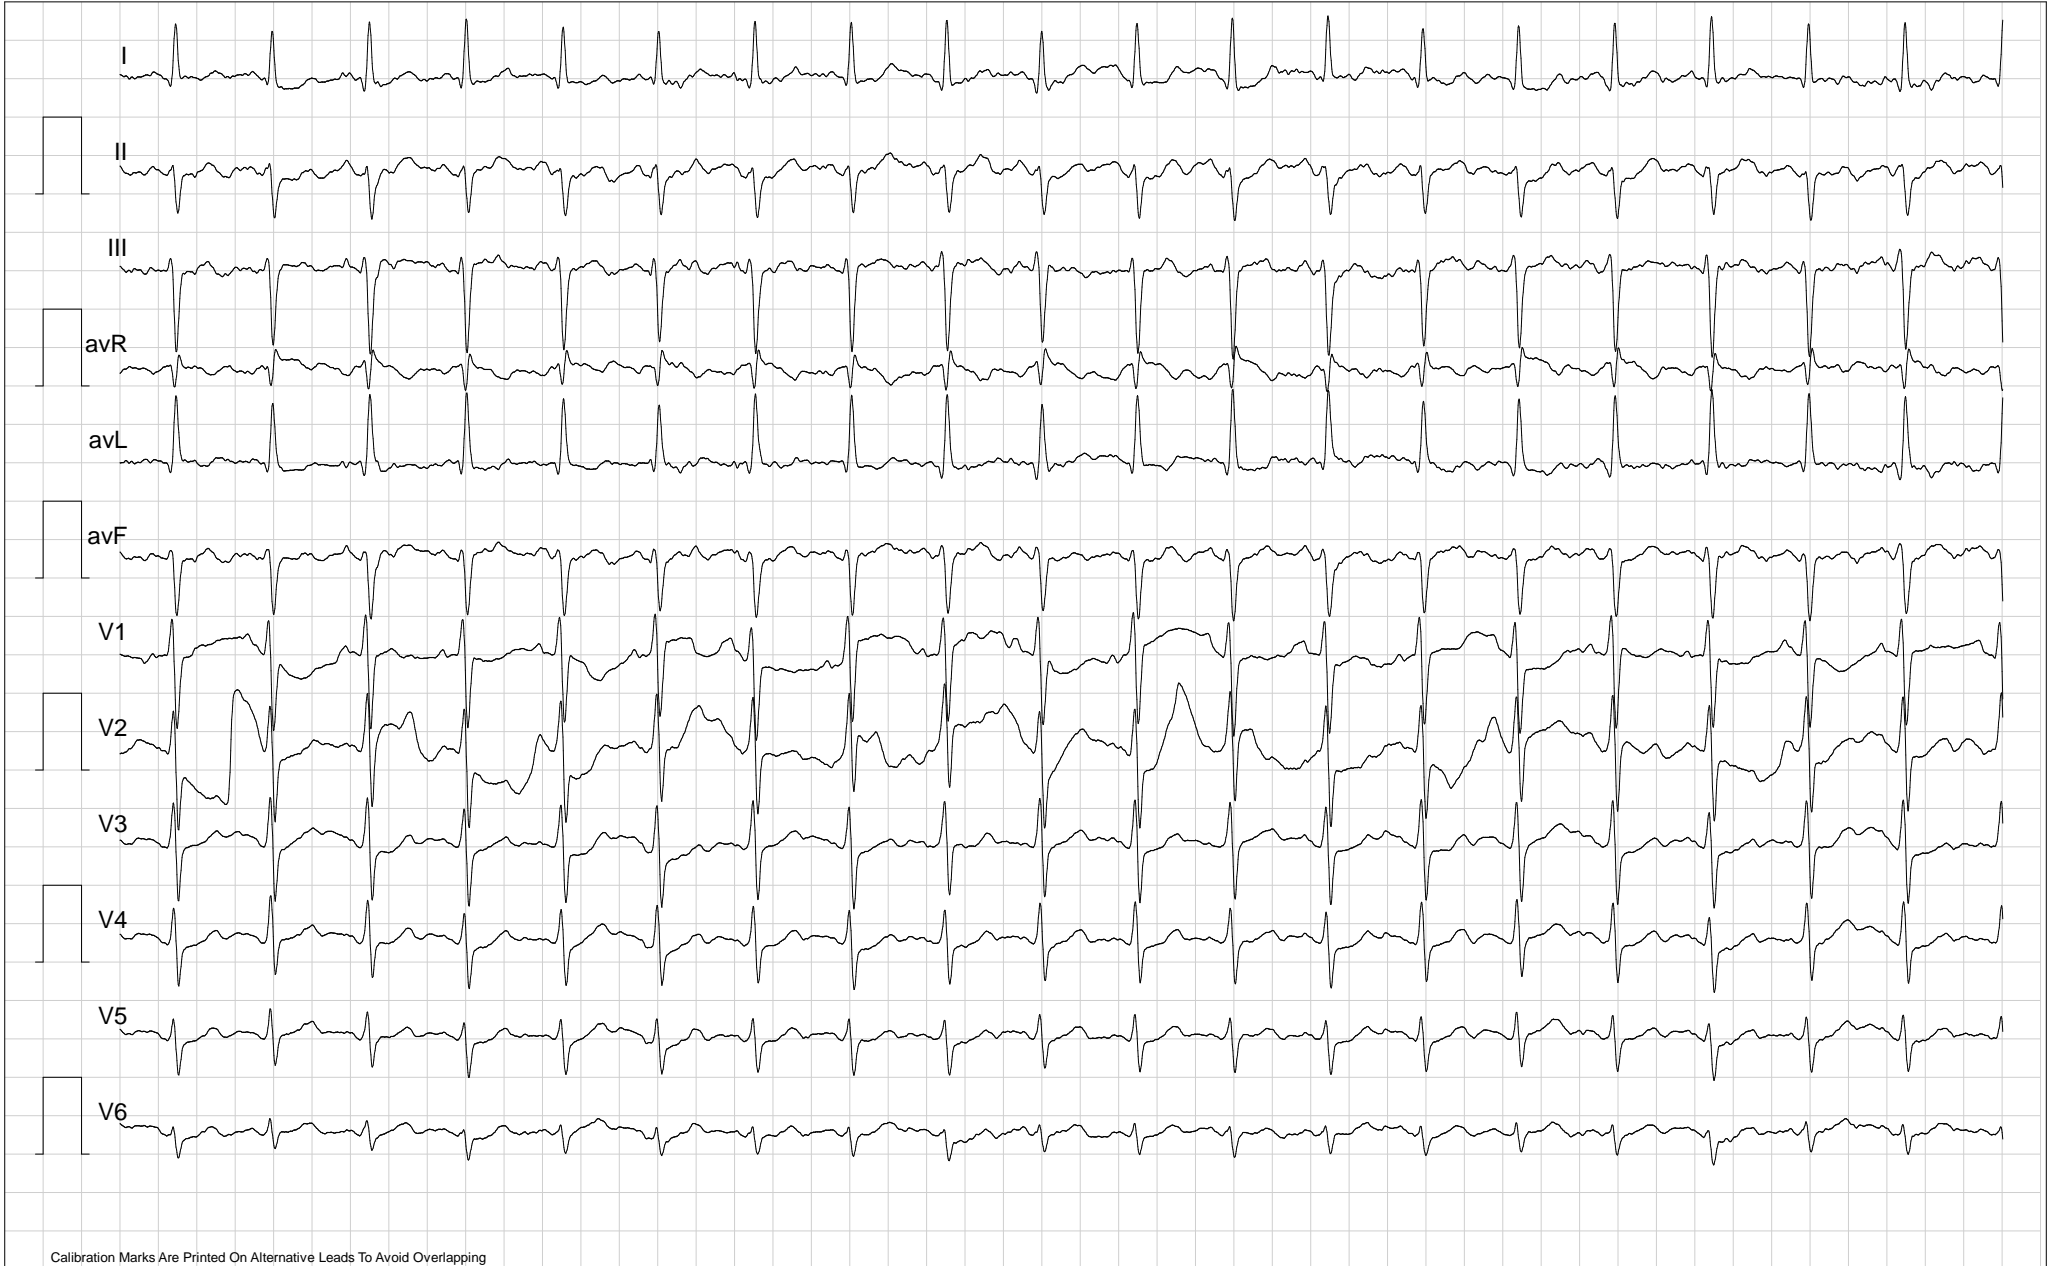


Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Date: 14 - 09 - 2024

METs : 1.5 HR : 108 Target HR : 67% of 162 BP : 155/100

ExTime : 12:35 1.1 mph 0.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz

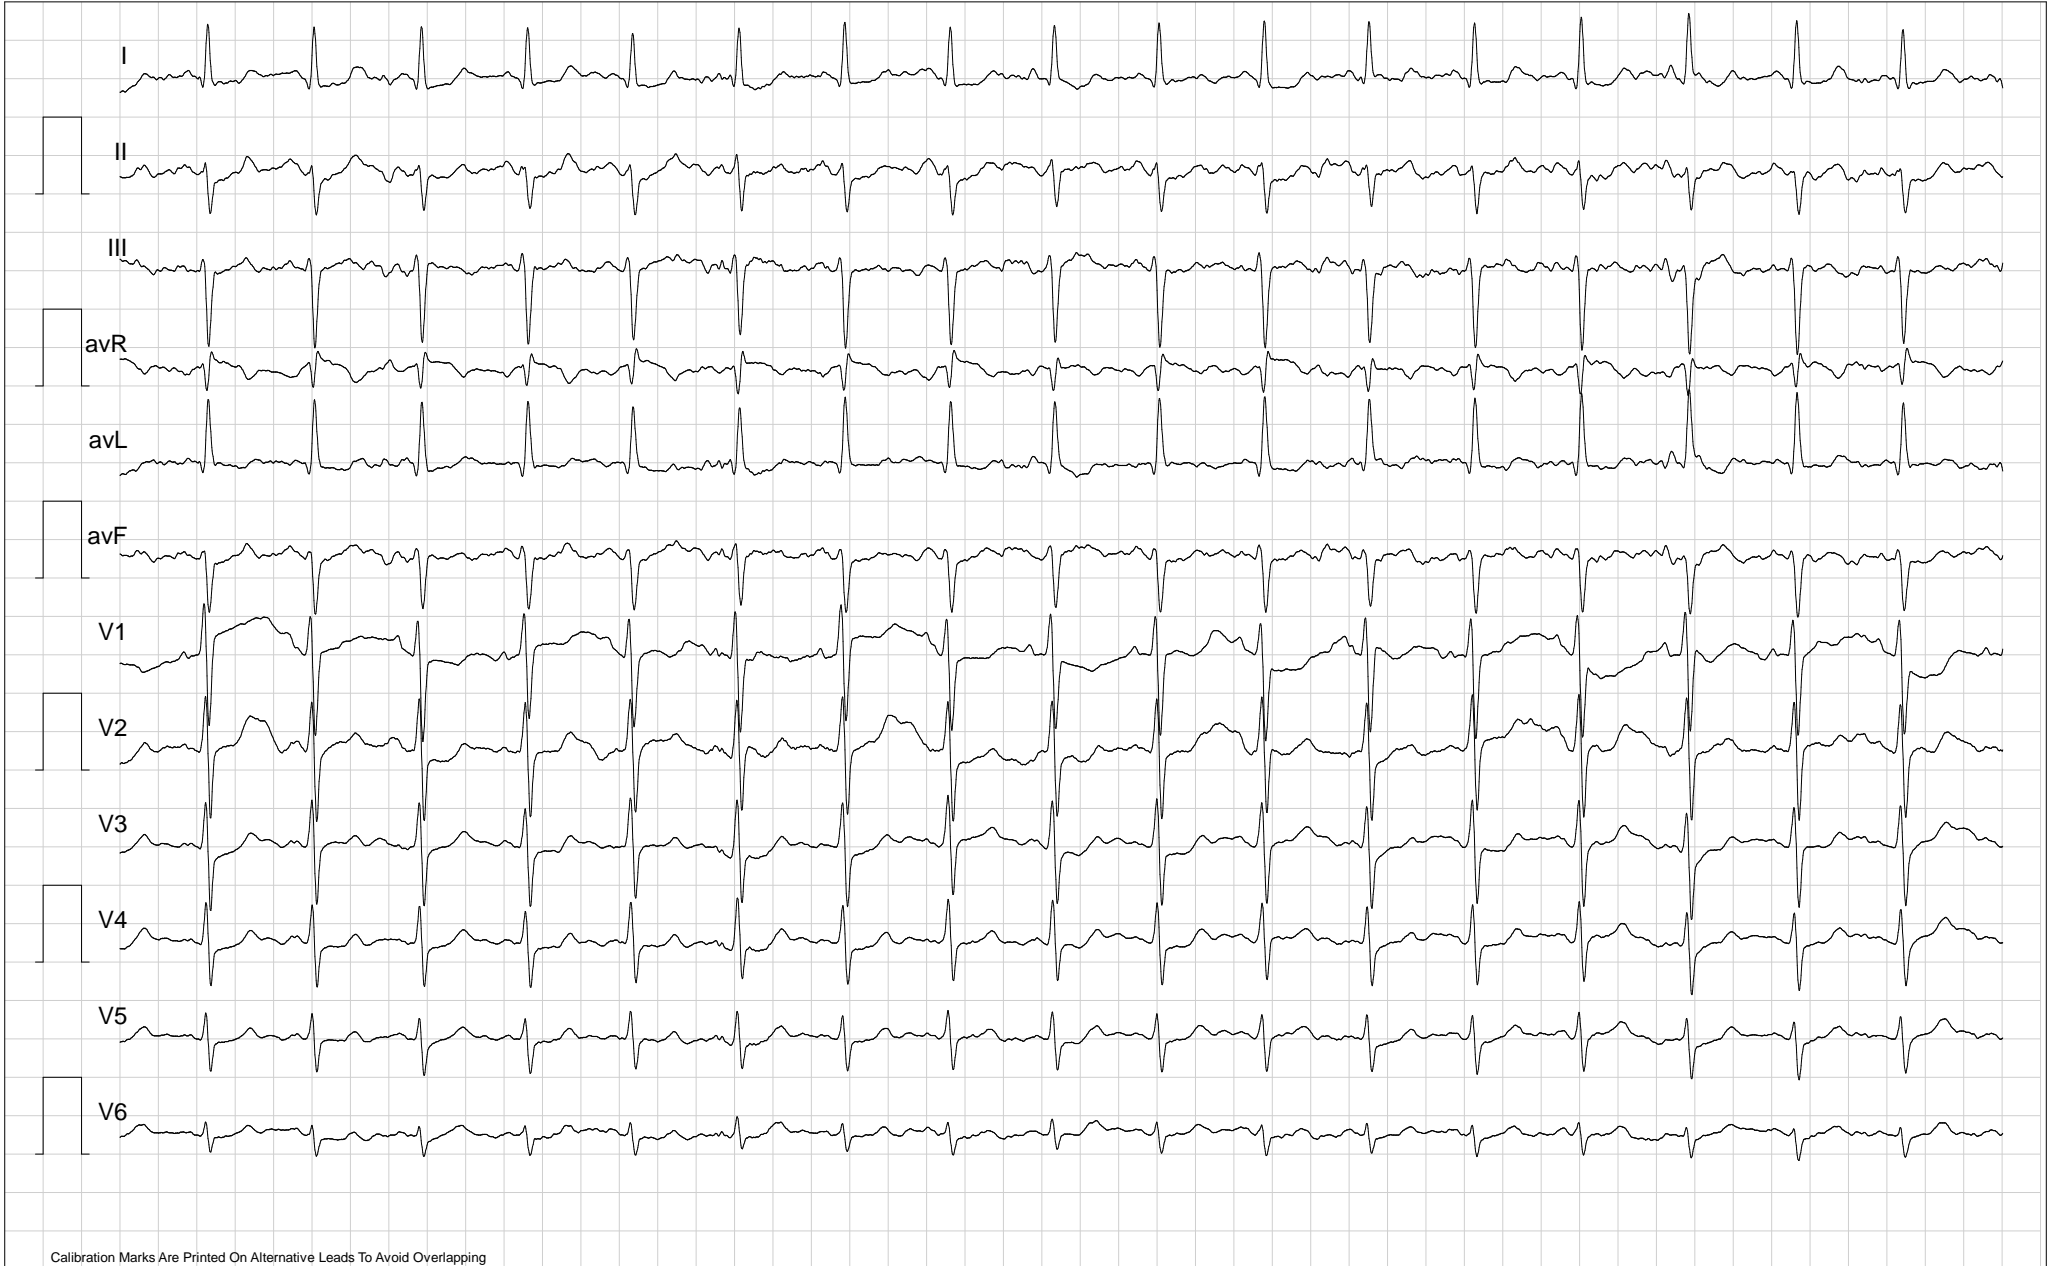

Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping






Date: 14 - 09 - 2024

METs : 1.0 HR : 103 Target HR : 64% of 162 BP : 150/95

ExTime : 12:35 1.1 mph 0.0 % 25 mm/Sec. 1.0 Cm/mV BLC On/ Notch On/ HF 0.05 Hz/LF 100 Hz

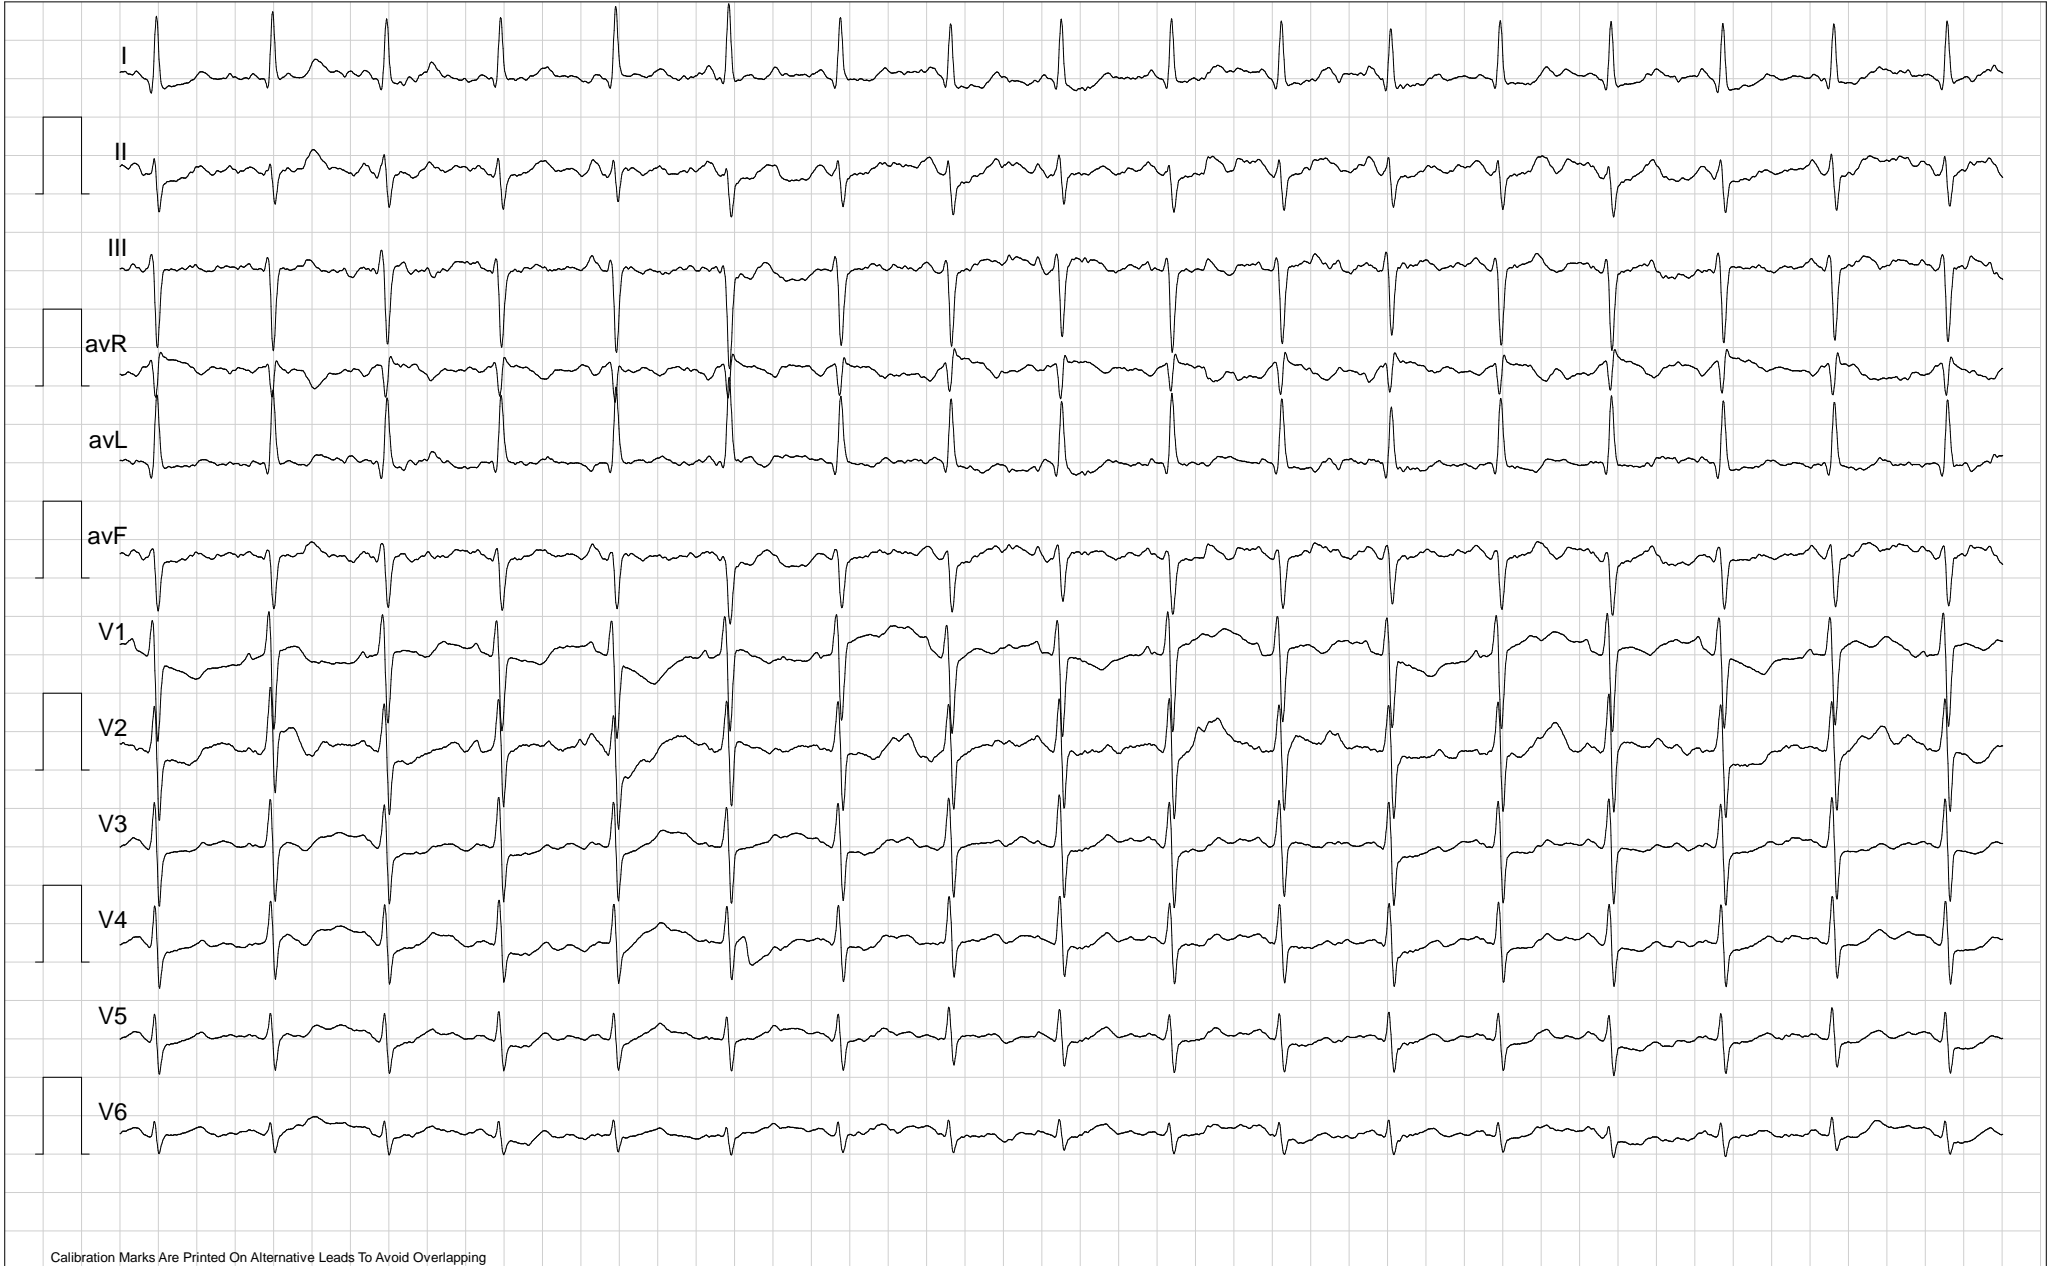

Calibration Marks Are Printed On Alternative Leads To Avoid Overlapping



Kartar Singh / 58 Yrs / Male / 0 Cm / 0 Kg

Time (Min.)	HR (bpm)	PR Int (mS)	QRS Wid (mS)	QRS Axis (Deg.)	QTC (mS)	P( $\mu$ V) (Max)	R( $\mu$ V) (Max)	S( $\mu$ V) (Min)	T( $\mu$ V) (Max)	Min. J ( $\mu$ V)	Leads for (J & PJ)	Min. Post JRR Var (%)	VEB (Counts)	Missed Beats (Counts)	
00 : 30	81	264	52	-31	469	242	857	-976	284	-401	III	-120	0.00	0	0
01 : 00	84	272	54	-28	480	-228	810	-934	322	112	I	-104	0.00	0	0
01 : 30	91	258	50	-34	529	456	810	-947	465	-425	III	-99	0.00	0	0
02 : 00	80	246	62	-34	204	279	768	-1000	-491	-616	V2	-441	0.00	0	0
02 : 30	88	252	50	-27	488	234	911	-1023	337	-185	V6	-123	0.00	0	0
03 : 00	90	252	50	-51	331	260	755	-983	-413	-204	I	-389	0.00	0	0
03 : 30	92	238	50	-27	429	401	896	-993	450	-456	III	-156	0.00	0	0
04 : 00	95	244	50	-29	109	511	860	-960	510	-774	V2	-371	0.00	0	0
04 : 30	93	238	48	-31	116	592	836	-982	552	-641	V2	-230	0.00	0	0
05 : 00	93	226	50	-50	138	293	777	-980	-706	-524	V2	-717	0.00	0	0
05 : 30	93	214	52	-40	155	701	744	-932	784	-51	I	-196	0.00	0	0
06 : 00	100	220	50	-33	139	340	791	-938	-342	-670	V2	-305	0.00	0	0
06 : 30	106	88	68	-34	277	-199	781	-910	-274	-572	V2	-169	0.00	0	0
07 : 00	109	184	52	-29	474	615	847	-950	582	-783	V2	-362	0.00	0	0
07 : 30	113	176	52	-24	475	372	829	-945	431	-783	V2	-362	0.00	0	0
08 : 00	114	92	50	-51	446	592	887	-1091	502	-583	II	-170	0.00	0	0
08 : 30	116	92	50	-24	446	518	839	-939	919	-247	V4	-109	0.00	0	0
09 : 00	116	92	50	-30	446	465	817	-986	-456	-387	II	-83	0.00	0	0
09 : 30	124	154	50	-36	140	-211	812	-975	-302	-457	V1	-297	0.00	0	0
10 : 00	127	124	100	-37	384	345	846	-1075	694	-186	V6	-82	0.00	0	0
10 : 30	128	152	50	-30	414	510	795	-1004	731	-701	V2	-429	0.00	0	0
11 : 00	129	152	52	-37	457	-556	825	-969	-596	-738	V2	-408	0.00	0	0
11 : 30	126	152	50	-32	387	-987	871	-996	-1112	-751	V2	-581	0.00	0	0
12 : 00	132	142	50	-26	430	314	810	-977	-447	-273	V6	-71	0.00	0	0
12 : 30	138	102	50	-39	332	346	757	-1067	456	83	avL	-218	0.00	0	0



Kartar Singh / 58 Yrs / Male / 0 Cm / 0 Kg

Time (Min.)	HR (bpm)	PR Int (mS)	QRS Wid (mS)	QRS Axis (Deg.)	QTC (mS)	P( $\mu$ V) (Max)	R( $\mu$ V) (Max)	S( $\mu$ V) (Min)	T( $\mu$ V) (Max)	Min. J ( $\mu$ V)	Leads for (J & PJ)	Min. Post JRR Var ( $\mu$ V)	JRR Var (%)	VEB (Counts)	Missed Beats (Counts)
13 : 00	124	170	50	-41	145	182	800	-978	-257	-15	I	-77	0.00	0	0
13 : 30	116	178	50	-39	137	210	828	-1033	-318	238	avL	-73	0.00	0	0
14 : 00	111	184	48	-39	147	166	802	-1052	-288	28	I	-73	0.00	0	0
14 : 30	106	186	52	-36	448	156	807	-1008	200	-44	I	-78	0.00	0	0
15 : 00	103	122	52	-36	428	183	876	-1017	-319	39	I	-84	0.00	0	0
15 : 30	102	126	48	-34	142	148	852	-996	-315	-763	V2	-71	0.00	0	0
16 : 00	103	196	50	-33	165	194	851	-976	-260	-673	V2	-85	0.00	0	0
16 : 30	102	124	50	-34	148	163	845	-975	-301	27	I	-58	0.00	0	0

# Allengers

E-Mail:

Report



**Kartar Singh / 58 Yrs / M / 0 Cms / 0 Kg**

**Date: 14 - 09 - 2024**

Stage	Time	Duration	Speed(mph)	Elevation	METs	Rate	% THR	BP	RPP	PVC	Comments
ExStart	00:01	0:01	01.7	10.0	01.1	077	48 %	---/---	000	00	
BRUCE Stage 1	03:01	3:00	01.7	10.0	04.7	089	55 %	135/86	120	00	
BRUCE Stage 2	06:01	3:00	02.5	12.0	07.1	095	59 %	140/90	133	00	
BRUCE Stage 3	09:01	3:00	03.4	14.0	10.2	115	71 %	145/95	166	00	
BRUCE Stage 4	12:01	3:00	04.2	16.0	13.5	128	79 %	155/100	198	00	
PeakEx	12:36	0:35	05.0	18.0	13.8	136	84 %	155/100	210	00	
Recovery	13:36	1:00	01.1	00.0	07.5	119	73 %	160/105	190	00	
Recovery	14:36	2:00	01.1	00.0	01.5	108	67 %	155/100	167	00	
Recovery	16:36	4:00	01.1	00.0	01.0	103	64 %	150/95	154	00	
Recovery	16:49	4:12	01.1	00.0	01.0	102	63 %	150/95	153	00	

## FINDINGS :

**Exercise Time** : 12:35  
**Max HR Attained** : 136 bpm 84% of Target 162  
**Max BP Attained** : 160/105 (mm/Hg)  
**Max WorkLoad Attained** : 13.8 Good response to induced stress  
**Max ST Dep Lead & Avg ST Value** : V2 & -7.2 mm in Stage 4  
**Test End Reasons** : Test Complete , Feeling Uncomfortable

## REPORT :

**Doctor : self**