



LABORATORY REPORT

Name : Ms. Charvi Bhagat	Reg. No : 312101148
Sex/Age : Female/36 Years	Reg. Date : 23-Dec-2023 09:13 AM
Ref. By :	Collected On :
Client Name : Mediwheel	Report Date : 23-Dec-2023 01:37 PM

Medical Summary

GENERAL EXAMINATION

Height (cms) :152

Weight (kgs) :76.0

Blood Pressure : 108/68mmHg

Pulse : 71/Min

No Clubbing/Cynosis/Pallor/PedelOedem

Systemic Examination:

Cardio vascular System - S1,S2 Normal, No Murmur


Respiratory system - AEBE

Central Nervous System - No FND


Abdomen - Soft, Non Tender, No Organomegaly

Epilepsy – N/A

This is an electronically authenticated report



Dr. Jay Soni
M.D, GENERAL MEDICINE





भारत सरकार




Charvi Bhagat
DOB: 29-03-1987
Gender: Female



4297 7639 0582

आधार - आम आदमी का अधिकार

Dr. Jay Soni
M.D. (General Medicine)
Reg. No.: G-23899



Handwritten signature and date: 23/12/2025
Handwritten number: 9712990288



भारतीय विशिष्ट पहचान प्राधिकरण
INDIA

W/O: हीरेन भगत, 27, श्रेणिक पार्क
सोसायटी, प्रगति नगर सामे,
नवयुग कॉलेज पाछा, सुरत सिटी,
नवयुग कॉलेज, सुरत सिटी, सुरत,
गुजरात, 395009

Address:
W/o: Hiren Bhagat, 27, Shrenik
Park Society, Opp. Pragati Nagar,
Behind Navyug College, Surat City,
Navyug College, Surat City, Surat,
Gujarat, 395009



1947
1800 300 1947

help@uidai.gov.in

www.uidai.gov.in

P.O. Box No. 1947,
Bengaluru-560 001



TEST REPORT

Reg. No : 312101148	Ref Id :	Collected On : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat		Reg. Date : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female	Pass. No. :	Tele No. : 9712990288
Ref. By :		Dispatch At :
Sample Type : EDTA		Location : CHPL

Parameter	Results	Unit	Biological Ref. Interval
-----------	---------	------	--------------------------

COMPLETE BLOOD COUNT (CBC)

Hemoglobin (Colorimetric method)	13.5	g/dL	12.5 - 16
Hematocrit (Calculated)	L 37.80	%	40 - 50
RBC Count (Electrical Impedance)	L 4.54	million/cmm	4.73 - 5.5
MCV (Calculated)	83.1	fL	83 - 101
MCH (Calculated)	29.7	Pg	27 - 32
MCHC (Calculated)	H 35.7	%	31.5 - 34.5
RDW (Calculated)	L 10.8	%	11.5 - 14.5
WBC Count Flowcytometry with manual Microscopy	5780	/cmm	4000 - 10000
MPV (Calculated)	9.5	fL	6.5 - 12.0

<u>DIFFERENTIAL WBC COUNT</u>	[%]	EXPECTED VALUES	[Abs]	EXPECTED VALUES
Neutrophils (%)	49	% 40 - 80	2832 /cmm	2000 - 7000
Lymphocytes (%)	40	% 20 - 40	2312 /cmm	1000 - 3000
Eosinophils (%)	02	% 0 - 6	520 /cmm	200 - 1000
Monocytes (%)	09	% 2 - 10	116 /cmm	20 - 500
Basophils (%)	00	% 0 - 2	0 /cmm	0 - 100

PERIPHERAL SMEAR STUDY


RBC Morphology Normocytic and Normochromic.
WBC Morphology Normal

PLATELET COUNTS

Platelet Count (Electrical Impedance) 295000 /cmm 150000 - 450000
Electrical Impedance
Platelets Platelets are adequate with normal morphology.
Parasites Malarial parasite is not detected.
Comment -

This is an electronically authenticated report.

* This test has been out sourced.

Approved By : 
Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 09:57 AM
Page 1 of 11



TEST REPORT

Reg. No	: 312101148	Ref Id	:	Collected On	: 23-Dec-2023 09:13 AM
Name	: Ms. Charvi Bhagat			Reg. Date	: 23-Dec-2023 09:13 AM
Age/Sex	: 36 Years / Female	Pass. No.	:	Tele No.	: 9712990288
Ref. By	:			Dispatch At	:
Sample Type	: EDTA			Location	: CHPL

Parameter	Result	Unit	Biological Ref. Interval
-----------	--------	------	--------------------------

HEMATOLOGY

BLOOD GROUP & RH

Specimen: EDTA and Serum; Method: Forward Reverse Tube Agglutination

ABO	"B"
Rh (D)	Negative
Note	-

ERYTHROCYTE SEDIMENTATION RATE [ESR]


ESR 1 hour <i>Westergreen method</i>	05	mm/hr	ESR AT 1 hour : 3-12
--	----	-------	----------------------

ERYTHRO SEDIMENTATION RATE, BLOOD -

Erythrocyte sedimentation rate (ESR) is a non-specific phenomena and is clinically useful in the diagnosis and monitoring of disorders associated with an increased production of acute phase reactants. The ESR is increased in pregnancy from about the 3rd month and returns to normal by the 4th week post partum. ESR is influenced by age, sex, menstrual cycle and drugs (eg. corticosteroids, contraceptives). It is especially low (<1mm) in polycythaemia, hypofibrinogenemia or congestive cardiac failure and when there are abnormalities of the red cells such as poikilocytosis, spherocytosis or sickle cells.

This is an electronically authenticated report.

* This test has been outsourced.

Approved By : 
Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 02:14 PM
Page 2 of 11



TEST REPORT

Reg. No : 312101148 **Ref Id** : **Collected On** : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat **Reg. Date** : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female **Pass. No.** : **Tele No.** : 9712990288
Ref. By : **Dispatch At** :
Sample Type : Serum,Flouride PP **Location** : CHPL

Parameter **Result** **Unit** **Biological Ref. Interval**

BIO - CHEMISTRY

Fasting Blood Sugar (FBS) 92.50 mg/dL 70 - 110
GOD-POD Method

Post Prandial Blood Sugar (PPBS) 106.2 mg/dL 70 - 140
GOD-POD Method

This is an electronically authenticated report.
* This test has been out sourced.

Deep
Approved By : Dr. Deep Patel
MD (Pathology)
Approved On : 23-Dec-2023 01:09 PM
Page 3 of 11



TEST REPORT

Reg. No : 312101148	Ref Id :	Collected On : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat		Reg. Date : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female	Pass. No. :	Tele No. : 9712990288
Ref. By :		Dispatch At :
Sample Type : Serum		Location : CHPL


Parameter	Result	Unit	Biological Ref. Interval
-----------	--------	------	--------------------------

Lipid Profile

Cholesterol	193.00	mg/dL	Desirable: <200.0 Borderline High: 200-239 High: >240.0
<i>Enzymatic, colorimetric method</i>			
Triglyceride	52.80	mg/dL	Normal: <150.0 Borderline: 150-199 High: 200-499 Very High : > 500.0
<i>Enzymatic, colorimetric method</i>			
HDL Cholesterol	63.20	mg/dL	Low: <40 High: >60
<i>Accelerator selective detergent method</i>			
LDL	119.24	mg/dL	Optimal: <100.0 Near Optimal: 100-129 Borderline High: 130-159 High : 160-189 Very High : >190.0
<i>Calculated</i>			
VLDL	10.56	mg/dL	15 - 35
<i>Calculated</i>			
LDL / HDL RATIO	1.89		0 - 3.5
<i>Calculated</i>			
Cholesterol /HDL Ratio	3.05		0 - 5.0
<i>Calculated</i>			

This is an electronically authenticated report.

* This test has been out sourced.

Approved By : 
Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 10:44 AM
Page 4 of 11



TEST REPORT

Reg. No : 312101148	Ref Id :	Collected On : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat		Reg. Date : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female	Pass. No. :	Tele No. : 9712990288
Ref. By :		Dispatch At :
Sample Type : Serum		Location : CHPL


Parameter	Result	Unit	Biological Ref. Interval
-----------	--------	------	--------------------------

LFT WITH GGT

Total Protein	6.47	gm/dL	1Day: 3.4-5.0 1Day to 1Month: 4.6-6.8 2 to 12Months: 4.8-7.6 ≥1Year : 6.0-8.0 Adults : 6.6-8.7
<i>Biuret Reaction</i>			
Albumin	4.58	g/dL	0 - 4 days: 2.8 - 4.4 4 days - 14 yrs: 3.8 - 5.4 14 - 19 yrs: 3.2 - 4.5 20 - 60 yrs : 3.5 - 5.2 60 - 90 yrs : 3.2 - 4.6 > 90 yrs: 2.9 - 4.5
<i>By Bromocresol Green</i>			
Globulin (Calculated)	1.89	g/dL	2.3 - 3.5
A/G Ratio (Calculated)	2.42		0.8 - 2.0
SGOT	15.80	U/L	0 - 40
<i>UV without P5P</i>			
SGPT	13.80	U/L	0 - 40
<i>UV without P5P</i>			
Alakaline Phosphatase	39.2	IU/l	42 - 98
<i>P-nitrophenyl phosphatase-AMP Buffer, Multiple-point rate</i>			
Total Bilirubin	0.82	mg/dL	0.3 - 1.2
<i>Vanadate Oxidation</i>			
Direct Bilirubin	0.15	mg/dL	0.0 - 0.4
<i>Vanadate Oxidation</i>			
Indirect Bilirubin	0.67	mg/dL	0.0 - 1.1
<i>Calculated</i>			
GGT	12.50	U/L	< 38
<i>SZASZ Method</i>			

This is an electronically authenticated report.

* This test has been out sourced.

Approved By :  Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 10:48 AM
Page 5 of 11



TEST REPORT

Reg. No : 312101148 **Ref Id** :
Name : Ms. Charvi Bhagat
Age/Sex : 36 Years / Female **Pass. No.** :
Ref. By :
Sample Type : Serum

Collected On : 23-Dec-2023 09:13 AM
Reg. Date : 23-Dec-2023 09:13 AM
Tele No. : 9712990288
Dispatch At :
Location : CHPL

Parameter	Result	Unit	Biological Ref. Interval
-----------	--------	------	--------------------------

BIO - CHEMISTRY

Uric Acid <i>Enzymatic, colorimetric method</i>	2.54	mg/dL	2.6 - 6.0
Creatinine <i>Enzymatic Method</i>	0.83	mg/dL	0.6 - 1.1
BUN <i>UV Method</i>	10.50	mg/dL	6.0 - 20.0

This is an electronically authenticated report.

* This test has been out sourced.

Deep
Approved By : Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 10:31 AM
Page 6 of 11


TEST REPORT

Reg. No : 312101148	Ref Id :	Collected On : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat		Reg. Date : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female	Pass. No. :	Tele No. : 9712990288
Ref. By :		Dispatch At :
Sample Type : EDTA		Location : CHPL

Parameter	Result	Unit	Biological Ref. Interval
-----------	--------	------	--------------------------

HEMOGLOBIN A1 C ESTIMATION

Specimen: Blood EDTA

*Hb A1C	4.9	% of Total Hb	Normal : < 5.7 % Pre-Diabetes : 5.7 % - 6.4 % Diabetes : 6.5 % or higher
---------	-----	---------------	--

Boronate Affinity with Fluorescent Quenching

Mean Blood Glucose	93.93	mg/dL
--------------------	-------	-------

Calculated
Degree of Glucose Control Normal Range:

Poor Control >7.0% *

Good Control 6.0 - 7.0 %**Non-diabetic level < 6.0 %

* High risk of developing long term complication such as retinopathy, nephropathy, neuropathy, cardiopathy, etc.

* Some danger of hypoglycemic reaction in Type I diabetics.

* Some glucose intolerant individuals and "subclinical" diabetics may demonstrate HbA1c levels in this area.

EXPLANATION :-

*Total haemoglobin A1 c is continuously synthesised in the red blood cell through its 120 days life span. The concentration of HBA1c in the cell reflects the average blood glucose concentration it encounters.

*The level of HBA1c increases proportionately in patients with uncontrolled diabetes. It reflects the average blood glucose concentration over an extended time period and remains unaffected by short-term fluctuations in blood glucose levels.

*The measurement of HbA1c can serve as a convenient test for evaluating the adequacy of diabetic control and in preventing various diabetic complications. Because the average half life of a red blood cell is sixty days, HbA1c has been accepted as a measurement which reflects the mean daily blood glucose concentration, better than fasting blood glucose determination, and the degree of carbohydrate imbalance over the preceding two months.

*It may also provide a better index of control of the diabetic patient without resorting to glucose loading procedures.

HbA1c assay Interferences:

*Erroneous values might be obtained from samples with abnormally elevated quantities of other Haemoglobins as a result of either their simultaneous elution with HbA1c(HbF) or differences in their glycation from that of HbA(HbS)

This is an electronically authenticated report.

* This test has been out sourced.

Deep

Approved By : Dr. Deep Patel
 MD (Pathology)

Approved On : 23-Dec-2023 04:18 PM

Page 7 of 11



TEST REPORT

Reg. No : 312101148 **Ref Id** : **Collected On** : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat **Reg. Date** : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female **Pass. No.** : **Tele No.** : 9712990288
Ref. By : **Dispatch At** :
Sample Type : Urine Spot **Location** : CHPL

Test	Result	Unit	Biological Ref. Interval
------	--------	------	--------------------------

URINE ROUTINE EXAMINATION

PHYSICAL EXAMINATION

Quantity	15 cc		
Colour	Pale Yellow		
Clarity	Clear		Clear

CHEMICAL EXAMINATION (BY REFLECTANCE PHOTOMETRIC)


pH	7.5		4.6 - 8.0
Sp. Gravity	1.005		1.001 - 1.035
Protein	Nil		Nil
Glucose	Nil		Nil
Ketone Bodies	Nil		Nil
Urobilinogen	Nil		Nil
Bilirubin	Nil		
Nitrite	Nil		Nil
Blood	Nil		Nil

MICROSCOPIC EXAMINATION (MANUAL BY MICROSCOPY)

Leucocytes (Pus Cells)	Nil		Nil
Erythrocytes (Red Cells)	Nil		Nil
Epithelial Cells	Occasional		Nil
Crystals	Absent		Absent
Casts	Absent		Absent
Amorphous Material	Absent		Absent
Bacteria	Absent		Absent
Remarks	-		

This is an electronically authenticated report.

* This test has been out sourced.

Approved By :  Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 10:52 AM
Page 8 of 11



TEST REPORT

Reg. No : 312101148	Ref Id :	Collected On : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat		Reg. Date : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female	Pass. No. :	Tele No. : 9712990288
Ref. By :		Dispatch At :
Sample Type : Serum		Location : CHPL

Parameter	Result	Unit	Biological Ref. Interval
-----------	--------	------	--------------------------

IMMUNOLOGY

THYROID FUNCTION TEST

T3 (Triiodothyronine) <small>CHEMILUMINESCENT MICROPARTICLE IMMUNOASSAY</small>	1.66	ng/mL	0.86 - 1.92
---	------	-------	-------------

Triiodothyronine (T3) is a hormone synthesized and secreted by the thyroid gland in response to the pituitary hormone TSH (thyroid stimulating hormone) and is regulated by a negative feedback mechanism involving the thyroid gland, pituitary gland and hypothalamus.

In the circulation, 99.7% of T3 is reversibly bond to transport proteins, primarily thyroxine-binding globulin (TBG) and to a lesser extent albumin and prealbumin. The remaining unbound T3 is free in the circulation and is metabolically active.

In hypothyroidism and hyperthyroidism, F T3 (free T3) levels parallel changes in total T3 levels. Measuring F T3 is useful in certain conditions such as normal pregnancy and steroid therapy, when altered levels of total T3 occur due to changes in T3 binding proteins, especially TBG.

T4 (Thyroxine) <small>CHEMILUMINECENT MICROPARTICLE IMMUNOASSAY</small>	9.10	µg/dL	3.2 - 12.6
---	------	-------	------------

Thyroxin (T4) is a hormone synthesized and secreted by the thyroid gland in response to the pituitary hormone TSH (thyroid stimulating hormone) and is regulated by a negative feedback mechanism involving the thyroid gland, pituitary gland and hypothalamus. In the circulation, 99.95% of T4 is reversibly bond to transport proteins, primarily thyroxine-binding globulin (TBG) and to a lesser extent albumin and thyroxine-binding prealbumin. The remaining unbound T4 is free in the circulation and is both metabolically active and a precursor to triiodothyronine (T3).


In hypothyroidism and hyperthyroidism, F T4 (free T4) levels parallel changes in total T4 levels. Measuring FT4 is useful in certain conditions such as normal pregnancy and steroid therapy, when altered levels of total T4 occur due to changes in T4 binding proteins, especially TBG.

Limitations:

1. The anticonvulsant drug phenytoin may interfere with total and F T4 levels due to competition for TBG binding sites.
2. F T4 values may be decreased in patients taking carbamazepine.
3. Thyroid autoantibodies in human serum may interfere and cause falsely elevated F T4 results.

This is an electronically authenticated report.

* This test has been out sourced.

Approved By : 
Dr. Deep Patel
MD (Pathology)

Approved On : 23-Dec-2023 10:52 AM
Page 10 of 1



TEST REPORT

Reg. No : 312101148	Ref Id :	Collected On : 23-Dec-2023 09:13 AM
Name : Ms. Charvi Bhagat		Reg. Date : 23-Dec-2023 09:13 AM
Age/Sex : 36 Years / Female	Pass. No. :	Tele No. : 9712990288
Ref. By :		Dispatch At :
Sample Type : Serum		Location : CHPL

TSH **7.940** μ IU/ml 0.35 - 5.50
CHEMILUMINECENT MICROPARTICLE IMMUNOASSAY

Thyroid stimulating hormone (TSH) is synthesized and secreted by the anterior pituitary in response to a negative feedback mechanism involving concentrations of FT3 (free T3) and FT4 (free T4). Additionally, the hypothalamic tripeptide, thyrotropin-releasing hormone (TRH), directly stimulates TSH production. TSH stimulates thyroid cell production and hypertrophy, also stimulate the thyroid gland to synthesize and secrete T3 and T4. Quantification of TSH is significant to differentiate primary (thyroid) from secondary (pituitary) and tertiary (hypothalamus) hypothyroidism. In primary hypothyroidism, TSH levels are significantly elevated, while in secondary and tertiary hypothyroidism, TSH levels are low.

TSH levels During Pregnancy :

First Trimester : 0.1 to 2.5 μ IU/mL

Second Trimester : 0.2 to 3.0 μ IU/mL


Third trimester : 0.3 to 3.0 μ IU/mL

Reference : Carl A. Burtis, Edward R. Ashwood, David E. Bruns. Tietz Textbook of Clinical Chemistry and Molecular Diagnostics. 5th Edition. Philadelphia: WB Saunders, 2012:2170

----- End Of Report -----

This is an electronically authenticated report.

* This test has been outsourced.


Approved By : **Dr. Deep Patel**
MD (Pathology)

Approved On : 23-Dec-2023 10:52 AM
Page 11 of 1



LABORATORY REPORT

Name : Ms. Charvi Bhagat	Reg. No : 312101148
Sex/Age : Female/36 Years	Reg. Date : 23-Dec-2023 09:13 AM
Ref. By :	Collected On :
Client Name : Mediwheel	Report Date : 23-Dec-2023 01:11 PM


Electrocardiogram

Findings


Normal Sinus Rhythm.

Within Normal Limit.

This is an electronically authenticated report



Dr. Jay Soni
M.D, GENERAL MEDICINE



Page 1 of 5

CHARVI
BHARGAVI

19

Female

36 years

152 cm / 76 kg

HR 71/min

Px15: P 38
QRS 28
T 5

Intervals:

RR 844 ms

P 98 ms

PR 128 ms

QRS 74 ms

QT 398 ms

QTc 429 ms
(Bazett)

10 mm/mV




P (II) 0.11 mV

S (V1) -1.06 mV

R (V5) 0.60 mV

Sokol. 1.79 mV

10 mm/mV



10 mm/mV

25 mm/s

0.05-25 Hz FS0 SSF 585 28.12.2023 10:02:29

CURQVIS HEALTHCARE

PL-102p us 1.24 C

SCHILLER

Part No.2.157017M

CE 0123

L80




LABORATORY REPORT

Name :	Ms. Charvi Bhagat	Reg. No :	312101148
Sex/Age :	Female/36 Years	Reg. Date :	23-Dec-2023 09:13 AM
Ref. By :		Collected On :	
Client Name :	Mediwheel	Report Date :	23-Dec-2023 01:11 PM


2D Echo Colour Doppler

1. Mild concentric LVH.
2. Normal sized LA, LV, RA, RV.
3. Normal LV systolic function, LVEF: 60%.
4. No RWMA.
5. Reduced LV compliance.
6. All cardiac valves are structurally normal.
7. Mild MR, Trivial TR, Trivial PR, No AR.
8. Mild PAH, RVSP: 38 mm Hg.
9. IAS/IVS: Intact.
10. No clot/vegetation/pericardial effusion.
11. No coarctation of aorta.

This is an electronically authenticated report



Dr. Jay Soni
M.D, GENERAL MEDICINE



Name: Charvi Bhagat

M MODE FINDINGS:


MITRAL VALVE	OBSERVED	NORMAL VALUES	LV FUNCTION
Anterior leaflet	Normal		LVA(d) :
EF Slope		70-150mm/sec	LVL (d) :
Opening Amplitude			LVA(s) :
Posterior leaflet	Normal		LVL(s) :
E.P.S.S.		mm	LVV(d) :
Mitral Valve Prolapse	No		LVV(s) :
Vegetation	No		LVEF : 60%
TRICUSPID VALVE		LV COMPLIANCE	
Normal		Reduced LV Compliance	

PULMONARY VALVE	OBSERVED	NORMAL VALUES	MVO AREA
EF Slope		6-115 mm	By Planimetry :
A' Wave -			
Midsystolic notch -			By PHT :
Flutter -			
Other Findings			

DIMENSIONS:			AORTIC VALVE		
1. Lvd. (Diastole)	46 mm		Cuspal Opening	16mm	
2. Lvd. (Systole)	28 mm	24-42 mm	Closure line	Central	
3. RVID (Diastole)	13mm	7-23 mm	Eccentricity index	1	
4. IVS (Diastole)	11mm		Other findings	Absent	
5. IVS (Systole)	12mm				
6. LVPWT (Diastole)	11mm	6-11 mm			
7. LVPM (Systole)	12mm				
8. Aortic root	32 mm	22-37 mm			
9. Left Atrium:	36 mm	19-40 mm			
10. LVEF	60%				

COLOUR DOPPLER FINDINGS:

STRUCTURE	REGURG GRADING	VELOCITY1 m/sec Max/Mean	GRADIENT 5 Mm Hg Peak/Mean
MITRAL VALVE	Mild	0.90	3.30
TRICUSPID VALVE	Trivial	0.58	1.40
PULMONARY VALVE	Trivial	0.75	2.25
AORTIC	No	1.20	6.0





LABORATORY REPORT

Name :	Ms. Charvi Bhagat	Reg. No :	312101148
Sex/Age :	Female/36 Years	Reg. Date :	23-Dec-2023 09:13 AM
Ref. By :		Collected On :	
Client Name :	Mediwheel	Report Date :	23-Dec-2023 01:18 PM

X RAY CHEST PA

Both lung fields appear clear.

No evidence of any active infiltrations or consolidation.

Cardiac size appears within normal limits.

Both costo-phrenic angles appear free of fluid.


Both domes of diaphragm appear normal.

COMMENT: No significant abnormality is detected.

This is an electronically authenticated report



DR DHAVAL PATEL
Consultant Radiologist
MB,DMRE
Reg No:0494





LABORATORY REPORT

Name : Ms. Charvi Bhagat	Reg. No : 312101148
Sex/Age : Female/36 Years	Reg. Date : 23-Dec-2023 09:13 AM
Ref. By :	Collected On :
Client Name : Mediwheel	Report Date : 25-Dec-2023 09:28 AM

USG ABDOMEN

Liver appears normal in size & in echogenicity. No evidence of focal solid or cystic lesion seen. No evidence of dilatation of intra-hepatic biliary or portal radicals. PV is normal in caliber.

Gall bladder is normally distended. No evidence of calculus or mass seen. Gall bladder wall thickness appears normal.

Pancreas Visualized portion appears normal in size and echopattern. No evidence of focal lesions.

Spleen appears normal in size & echopattern.

Both kidneys are normal in size, shape and position. C.M. differentiation on both sides is maintained. No evidence of hydronephrosis, calculus or solid mass on either side.

Urinary bladder is partially distended. No evidence of calculus or mass lesion.

Uterus appears normal. No adnexal mass is seen.

No evidence of ascites.

No evidence of lymph adenopathy.


No evidence of dilated small bowel loops.

COMMENTS :


NO SIGNIFICANT ABNORMALITY DETECTED.

----- End Of Report -----

This is an electronically authenticated report



DR DHAVAL PATEL
Consultant Radiologist
MB,DMRE
Reg No:0494





LABORATORY REPORT

Name : Ms. Charvi Bhagat	Reg. No : 312101148
Sex/Age : Female/36 Years	Reg. Date : 23-Dec-2023 09:13 AM
Ref. By :	Collected On :
Client Name : Mediwheel	Report Date : 23-Dec-2023 02:37 PM

Eye Check - Up

No Eye Complaints

	Without Glasses	With Glasses
Right Eye	6/60	6/5
Left Eye	6/60	6/5

Near Vision: Right Eye - N/6, Left Eye - N/6

Fundus Examination - Within Normal Limits.

Color Vision : Normal


Comments: Normal

----- End Of Report -----

This is an electronically authenticated report



Dr Kejal Patel
MB,DO(Ophth)






LABORATORY REPORT

Name : Ms. Charvi Bhagat	Reg. No : 312101148
Sex/Age : Female/36 Years	Reg. Date : 23-Dec-2023 09:13 AM
Ref. By :	Collected On :
Client Name : Mediwheel	Report Date : 23-Dec-2023 02:37 PM

AUDIOGRAM

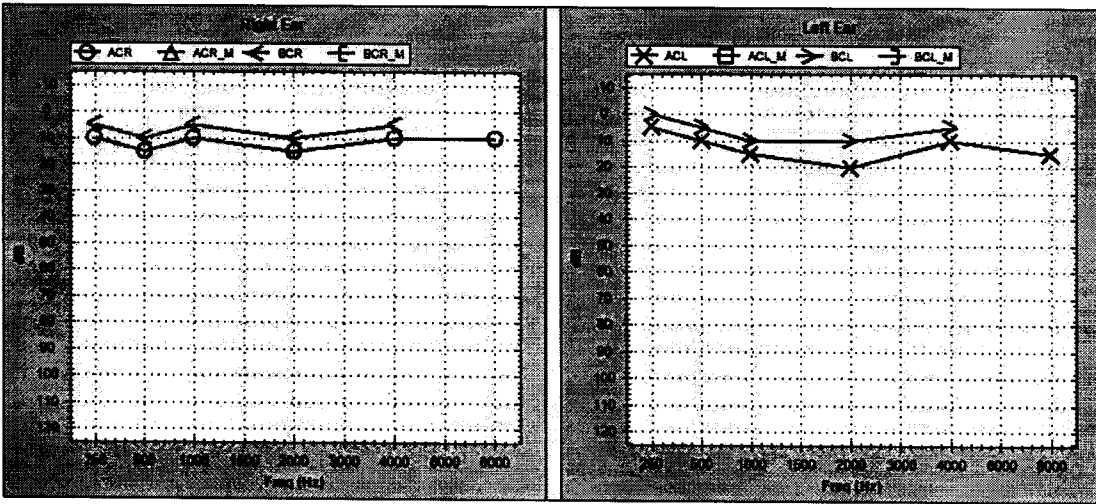


EAR	MODE	Air Conduction		Bone Conduction		Colour Code
		Masked	UnMasked	Masked	UnMasked	
LEFT		□	×	⌋	>	Blue
RIGHT		△	○	⌈	<	Red
NO RESPONSE : Add ↓ below the respective symbols						

Threshold In dB	RIGHT	LEFT
AIR CONDUCTION	10.5	10.5
BONE CONDUCTION		
SPEECH		

Comments: -Bilateral Hearing Sensitivity Within Normal Limits

----- End Of Report -----

This is an electronically authenticated report


Dr Kejal Patel
 MB,DO(Ophth)

